



~~Designation: E2562-07~~ Designation: E2562 - 12

Standard Test Method for Quantification of *Pseudomonas aeruginosa* Biofilm Grown with High Shear and Continuous Flow using CDC Biofilm Reactor¹

This standard is issued under the fixed designation E2562; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

~~1.1 This test method specifies the operational parameters required to grow a repeatable *Pseudomonas aeruginosa* biofilm under high shear~~

1.1 This test method specifies the operational parameters required to grow a reproducible (1):² *Pseudomonas aeruginosa* biofilm under high shear. The resulting biofilm is representative of generalized situations where biofilm exists under high shear rather than being representative of one particular environment.

~~1.2 This test method uses the Centers for Disease Control and Prevention (CDC) biofilm reactor. Biofilm Reactor. The CDC biofilm reactor Biofilm Reactor is a continuously stirred flow tank reactor (CSTR) with high wall shear. Although it was originally designed to model a potable water system for the evaluation of *Legionella pneumophila* (2), the reactor is versatile and may also be used for growing and/or characterizing biofilm of varying species (3 and 43-5).~~

~~1.3 This test method describes how to sample and analyze biofilm for viable cells. Biofilm population density is recorded as log₁₀ colony forming units per surface area.~~

~~1.4 Basic microbiology training is required to perform this test method.~~

~~1.5 The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only.~~

1.5 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

~~1.6 This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.~~

2. Referenced Documents

2.1 *ASTM Standards*:³

D5465 [Practice for Determining Microbial Colony Counts from Waters Analyzed by Plating Methods](#)

2.2 *Other Standards*: <http://www.astm.org/catalog/standards/sist/1a12be68-ba9e-48d4-8ecc-c9103f157113/astm-e2562-12>

~~Method 9050 C.1a Buffered Dilution Water Preparation Method 9050 C.1.a~~ Buffered Dilution Water Preparation according to Eaton et al (6)

3. Terminology

3.1 *Definitions*:

3.1.1 *biofilm, n*—microorganisms living in a ~~self-organized, cooperative~~ self-organized community attached to surfaces, interfaces, or each other, embedded in a matrix of extracellular polymeric substances of microbial origin, while exhibiting ~~an~~ altered phenotypes with respect to growth rate and gene transcription.

3.1.1.1 *Discussion*—Biofilms may be comprised of bacteria, fungi, algae, protozoa, viruses, or infinite combinations of these microorganisms. The qualitative characteristics of a biofilm (including, but not limited to, population density, taxonomic diversity, thickness, chemical gradients, chemical composition, consistency, and other materials in the matrix that are not produced by the biofilm microorganisms), are controlled by the physicochemical environment in which it exists.

3.1.2 *coupon, n*—biofilm sample surface.

¹ This test method is under the jurisdiction of ASTM Committee E35 on Pesticides, Antimicrobials, and Alternative Control Agents and is the direct responsibility of Subcommittee E35.15 on Antimicrobial Agents.

Current edition approved April 1, 2007. Published May 2007. DOI: 10.1520/E2562-07.

Current edition approved April 1, 2012. Published June 2012. Originally approved in 2007. Last previous edition approved in 2007 as E2562 - 07. DOI: 10.1520/E2562-12.

² The boldface numbers in parentheses refer to a list of references at the end of this standard.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

4. Summary of Test Method

4.1 This test method is used for growing a ~~repeatable~~reproducible *Pseudomonas aeruginosa* biofilm in a CDC ~~biofilm reactor~~Biofilm Reactor. The biofilm is established by operating the reactor in batch mode (no flow of the nutrients) for 24 h. A steady state population is reached while the reactor operates for an additional 24 h with continuous flow of the nutrients. The residence time of the nutrients in the reactor is set to select for biofilm growth, and is species and reactor parameter specific. During the entire 48 h, the biofilm is exposed to continuous fluid shear from the rotation of a baffled stir bar. Controlling the rate at which the baffle turns determines the intensity of the shear stress to which the coupons are exposed. At the end of the 48 h, biofilm accumulation is quantified by removing coupons from suspended rods, ~~scraping~~harvesting the biofilm from the coupon surface, disaggregating the clumps, and diluting and plating for viable cell enumeration.

5. Significance and Use

5.1 Bacteria that exist in biofilms are phenotypically different from suspended cells of the same genotype. Research has shown that biofilm bacteria are more difficult to kill than suspended bacteria (5, 7). Laboratory biofilms are engineered in growth reactors designed to produce a specific biofilm type. Altering system parameters will correspondingly result in a change in the biofilm. For example, research has shown that biofilm grown under high shear is more difficult to kill than biofilm grown under low shear (6, 8). The purpose of this test method is to direct a user in the laboratory study of a *Pseudomonas aeruginosa* biofilm by clearly defining each system parameter. This test method will enable an investigator to grow, sample, and analyze a *Pseudomonas aeruginosa* biofilm grown under high shear. The biofilm generated in the CDC ~~biofilm reactor~~Biofilm Reactor is also suitable for efficacy testing. After the 48 h growth phase is complete, the user may add the treatment in situ or harvest the coupons and treat them individually.

6. Apparatus

- 6.1 ~~Wooden Applicator Sticks, sterile.~~—sterile.
- 6.2 ~~Inoculating Loop.~~—Inoculating Loop.
- 6.3 ~~Petri Dish, 100 by 15 mm, plastic, sterile and empty to put beneath rod while sampling.~~—100- by 15-mm, plastic, sterile, and empty to put beneath rod while sampling.
- 6.4 ~~Culture Tubes and Culture Tube Closures, any—any with a volume capacity of 10 mL and a minimum diameter of 16 mm. Recommended size is 16- by 125-mm borosilicate glass with threaded opening.~~
- 6.5 ~~Pipetter—Continuously adjustable pipetter with volume capability.~~—capacity of 1 mL.
- 6.6 ~~Vortex—Any—any vortex that will ensure proper agitation and mixing of culture tubes.~~
- 6.7 ~~Homogenizer—Any—any that can mix at 20 500 ± 5000 r/min in a 5 to 10 mL volume.~~
- 6.8 ~~Homogenizer Probe—Any—any that can mix at 20 500 ± 5000 r/min in a 5- to 10-mL volume and can withstand autoclaving or other means of sterilization.~~
- 6.9 ~~Sonicator—Any noncavitating sonicating bath that operates at 50 to 60 Hz.~~—Sonicator—any cavitating sonicating bath that operates at 50 to 60 Hz.
- 6.10 ~~Bunsen Burner, used—used to flame inoculating loop and other instruments.~~
- 6.11 ~~Stainless Steel Hemostat Clamp, with curved tip.~~—with curved tip.

NOTE 1—Alternatively, a coupon holder⁴ may be used.

- 6.12 ~~Environmental Shaker, that—that can maintain a temperature of 35.36 ± 2°C.~~
 - 6.13 ~~Analytical Balance, sensitive to 0.01 g.~~—sensitive to 0.01 g.
 - 6.14 ~~Sterilizers—Any—any steam sterilizer that can produce the conditions of sterilization is acceptable.~~
 - 6.15 ~~Colony Counter—Any—any one of several types may be used, such as the Quebec, Buck, and Wolfhugel. A hand tally for the recording of the bacterial count is recommended if manual counting is done.~~
 - 6.16 ~~Peristaltic Pump—Pump head that can hold tubing with ID 3.1 mm and OD 3.2 mm.~~—pump head that can hold tubing with inner diameter 3.1 mm and outer diameter 3.2 mm.
 - 6.17 ~~Magnetic Stir Plate—Top plate 10.16 × 10.16 cm, that can rotate at 125 ± 60 r/min.~~
- NOTE 1—A digital stir plate is recommended. Digital Magnetic Stir Plate—top plate 10.16 × 10.16 cm, that can rotate at 125 ± 5 r/min.
- 6.18 ~~Silicone Tubing—Two—two sizes of tubing: one with ID inner diameter 3.1 mm and OD outer diameter 3.2 mm, and the other with ID inner diameter 7.9 mm and OD outer diameter 9.5 mm. Both sizes must withstand sterilization.~~
 - 6.19 ~~Norprene Tubing—inner diameter 3.1 mm and outer diameter 3.2 mm.~~
 - 6.20 ~~Glass Flow Break—Any that will connect with tubing of ID 3.1 mm and withstands sterilization.~~

⁴Eaton, A.D., Clesceri, L.S., Rice, E.W., Greenberg, A.E., (Eds.) *Standard Methods for the Examination of Water and Waste Water*, 21st Edition, American Public Health Association, American Water Works Association, Water Environment Federation, Washington D.C., 2005.

⁴The sole source of supply of the apparatus (coupon holder) known to the committee at this time is Biosurface Technologies, Corp., www.biofilms.biz. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. The user may also build the holder.

6.19.1—any that will connect with tubing of inner diameter 3.1 mm and withstand sterilization.

6.20.1 *Clamp*—Used to hold flow break, extension clamp with 0.5-cm minimum grip size.

6.19.26.20.2 *Clamp Stand—Height*—height no less than 76.2 cm, used with clamp to suspend glass flow break vertically and stabilize tubing above reactor.

6.20.21 *Reactor Components*.⁵

6.20.16.21.1 *Berzelius Pyrex or Kimax Borosilicate Glass Tall Beaker, 1000*—1000 mL without pour spout, 9.5 ± 0.5-cm diameter. Pyrex/Kimax ~~barbed~~ Barbed outlet spout added at 400 ± 20-mL mark. Angle the spout 30 to 45° to ensure drainage. Spout should accommodate flexible tubing with an ~~ID~~ inner diameter of 8 to 11 mm.

NOTE 2—The rods, described in rods (see 6.20.36.21.3) and baffle (see 6.20.56.21.6) will displace approximately 50 mL of liquid when system is completely assembled. Therefore, an outlet spout at the 400-mL mark will result in approximately a 350-mL operating volume. The user is encouraged to ~~should~~ confirm the actual liquid volume in the reactor, when the rods and baffle are in place and the stir plate is turned on, before use. The measured volume is used to calculate an exact pump flow rate.

6.20.26.21.2 *Reactor Top*—See—Fig. 1. Ultra-high molecular weight (UHMW) polyethylene top (10.1-cm diameter tapering to 8.33 cm) equipped with ~~3~~ a minimum of three holes accommodating 10-cm pieces of stainless steel or other rigid autoclavable tubing with ~~OD~~ outside diameter of 5 to 8 mm for media inlet, air exchange, and inoculation port. Center hole, 1.27-cm diameter, to accommodate the glass rod used to support the baffle assembly. Eight rod holes, 1.905-cm diameter, notched to accommodate stainless steel rod alignment pin (~~0.236-cm OD~~); (0.236-cm outside diameter).

6.20.36.21.3 *Polypropylene Rods*—See—Fig. 2. Eight polypropylene rods, 21.08-cm long, machined to hold three coupons (see 6.20.46.21.4) at the immersed end. Three 316 stainless steel set screws imbedded in side to hold coupons in place. Rods fit into holes in reactor top and lock into preformed notches with alignment pin.

6.20.46.21.4 *Twenty-four Cylindrical Polycarbonate Coupons*—with a diameter of 1.27 ± 0.013 cm, thickness of approximately 3.0 mm.

6.20.5

6.21.5 *Small Allen Wrench*, for loosening set screws.

6.20.6—*for loosening set screws.*

6.21.6 *Stir Blade Assembly (Baffled Stir Bar)*—See—Fig. 3. PTFE blade (5.61-cm) fitted into cylindrical PTFE holder (8.13-cm) and held in place with a magnetic stir bar (2.54-cm). PTFE holder fits onto a glass rod (15.8-cm), fitted into the reactor top. The glass rod is held in place with a compression fitting and acts as a support for the moving blade assembly.

6.21.6.22 *Carboys*—~~Two~~ two 20-L autoclavable carboys, to be used for waste and nutrients.

6.21.16.22.1 *Two Carboy Lids*—One carboy lid with at least two barbed fittings to accommodate tubing ID 3.1 mm (one for nutrient line and one for bacterial air vent). One carboy lid with at least two 1-cm holes bored in the same fashion (one for effluent waste and one for bacterial air vent).

ASTM E2562-12

⁵ The sole source of supply of the apparatus (CDC Biofilm reactor)Reactor known to the committee at this time is BioSurface Technologies, Corp. www.biosurface.biz. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. The user may also build the reactor.

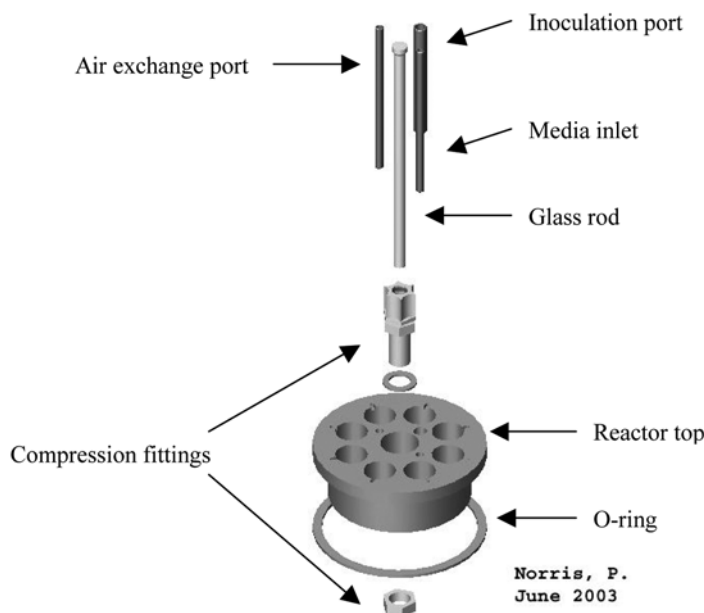


FIG. 1 Expanded Schematic of Reactor Top

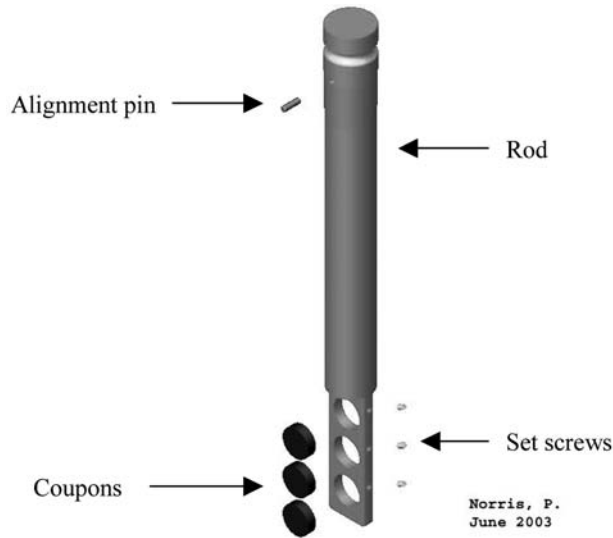


FIG. 2 Expanded Schematic of Rod and Coupons

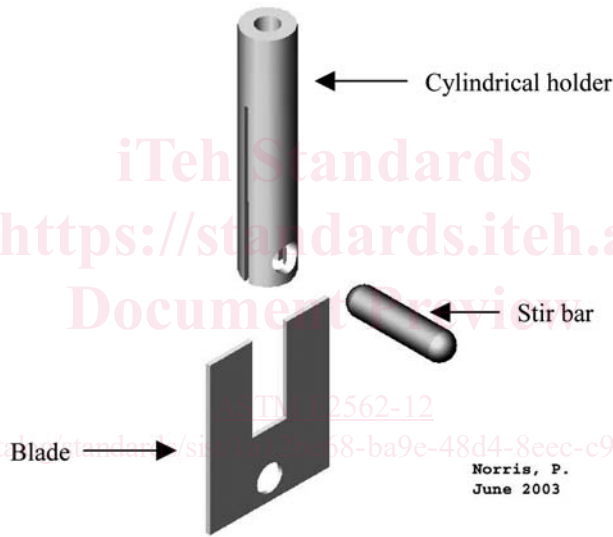


FIG. 3 Expanded Schematic of Baffled Stir Bar

NOTE 3—Carboy tops can be purchased with fittings.

6.21.2

6.22.2 *Bacterial Air Vent (Filter)*—Autoclavable, 0.2- μ m pore size, to be spliced into tubing on waste carboy, nutrient carboy, and reactor top; recommended diameter 37 mm.

6.226.23 Fig. 4 illustrates a schematic of the assembled system.

7. Reagents and Materials

7.1 *Purity of Water*—All reference to water as diluent or reagent shall mean distilled water or water of equal purity.

7.2 *Culture Media:*

7.2.1 *Bacterial Liquid Growth Broth*—Tryptic Soy Broth (TSB) is recommended.

7.2.2 *Bacterial Plating Medium*—R2A Agar is recommended.

NOTE 4—Two different TSB concentrations are used in the test method, 300 mg/L for the inoculum and batch reactor operation, and 100 mg/L for the continuous flow reactor operation.

7.2.2 *Bacterial Plating Medium*—R2A Agar is recommended.

7.3 *Buffered Water*—0.0425 g/L KH_2PO_4 distilled water, filter sterilized, and 0.405 g/L $\text{MgCl}_2 \cdot 6\text{H}_2\text{O}$ distilled water, filter sterilized (prepared according to Method 9050 C.1.a(6)).

8. Culture Preparation

8.1 *Pseudomonas aeruginosa* ATCC 700888 is the organism used in this test. Aseptically remove 3 to 5 an isolated colonies with