



Designation: D1929 – 12

Standard Test Method for Determining Ignition Temperature of Plastics¹

This standard is issued under the fixed designation D1929; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This standard has been approved for use by agencies of the Department of Defense.

1. Scope*

1.1 This fire test response test method² covers a laboratory determination of the flash ignition temperature and spontaneous ignition temperature of plastics using a hot-air furnace.

1.2 *Caution*—During the course of combustion, gases or vapors, or both, are evolved that have the potential to be hazardous to personnel.

1.3 *This standard is used to measure and describe the response of materials, products, or assemblies to heat and flame under controlled conditions, but does not by itself incorporate all factors required for fire-hazard or fire-risk assessment of the materials, products, or assemblies under actual fire conditions.*

1.4 *Fire testing is inherently hazardous. Adequate safeguards for personnel and property shall be employed in conducting these tests.*

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* Specific precautionary statements are given in 1.2 and 1.3.

NOTE 1—This test method and ISO 871-1996 are identical in all technical details.

¹ This test method is under the jurisdiction of ASTM Committee D20 on Plastics and is the direct responsibility of Subcommittee D20.30 on Thermal Properties.30.03).

Current edition approved April 15, 2012. Published June 2012. Originally approved in 1962. Last previous edition approved in 2011 as D1929 – 11. DOI:10.1520/D1929-12.

In 1996, this test method was totally revised to be technically equal to ISO 871-1996, and a specific air velocity is specified, which eliminates the need for approximations.

² The following reference may be of interest in connection with this test method: Stetchkin, N. P., "A Method and Apparatus for Determining the Ignition Characteristics of Plastics," *Journal of Research*, National Institute of Standards and Technology, Vol 43, No. 6, December 1949 (RP 2052), p. 591.

2. Referenced Documents

2.1 *ASTM Standards*:³

D618 Practice for Conditioning Plastics for Testing

E176 Terminology of Fire Standards

2.2 *International Standards*:⁴

ISO 871-1996 Plastics—Determination of Ignition Temperature Using a Hot-Air Furnace

ISO 5725 Precision of Test Methods—Determination of Repeatability and Reproducibility for Standard Test Methods by Interlaboratory Tests

IEC 584-2 Thermocouples—Part 2: Tolerances

3. Terminology

3.1 For definitions of terms relating to fire, see Terminology E176.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *flash ignition temperature (FIT)*—the minimum temperature at which, under specified test conditions, sufficient flammable gases are emitted to ignite momentarily upon application of a small external pilot flame.

3.2.2 *glowing combustion*—combustion of a material in the solid phase without flame but with emission of light from the combustion zone, caused by slow decomposition and carbonization at various points in the specimen, without general ignition occurring.

3.2.3 *spontaneous ignition temperature or self-ignition temperature (SIT)*—the minimum temperature at which the self-heating properties of the specimen lead to ignition or ignition occurs of itself, under specified test conditions, in the absence of any additional flame ignition source.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

⁴ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, <http://www.ansi.org>.

*A Summary of Changes section appears at the end of this standard

4. Significance and Use

4.1 Tests made under conditions herein prescribed can be of considerable value in comparing the relative ignition characteristics of different materials. Values obtained represent the lowest ambient air temperature that will cause ignition of the material under the conditions of this test. Test values are expected to rank materials according to ignition susceptibility under actual use conditions.

4.2 This test is not intended to be the sole criterion for fire hazard. In addition to ignition temperatures, fire hazards include other factors such as burning rate or flame spread, intensity of burning, fuel contribution, products of combustion, and others.

5. Apparatus

5.1 Hot-Air Ignition Furnace—A furnace similar to that shown in Fig. 1, consisting primarily of an electrical heating unit and specimen holder.

5.2 Furnace Tube—A vertical tube with an inside diameter of 100 ± 5 mm and a length of 230 ± 20 mm, made of a ceramic that will withstand at least 750°C . The vertical tube stands on the furnace floor, fitted with a plug for the removal of accumulated residue.

5.3 Inner Ceramic Tube—A ceramic tube that will withstand at least 750°C , with an inside diameter of 75 ± 5 mm, length of 230 ± 20 mm, and thickness of approximately 3 mm, placed

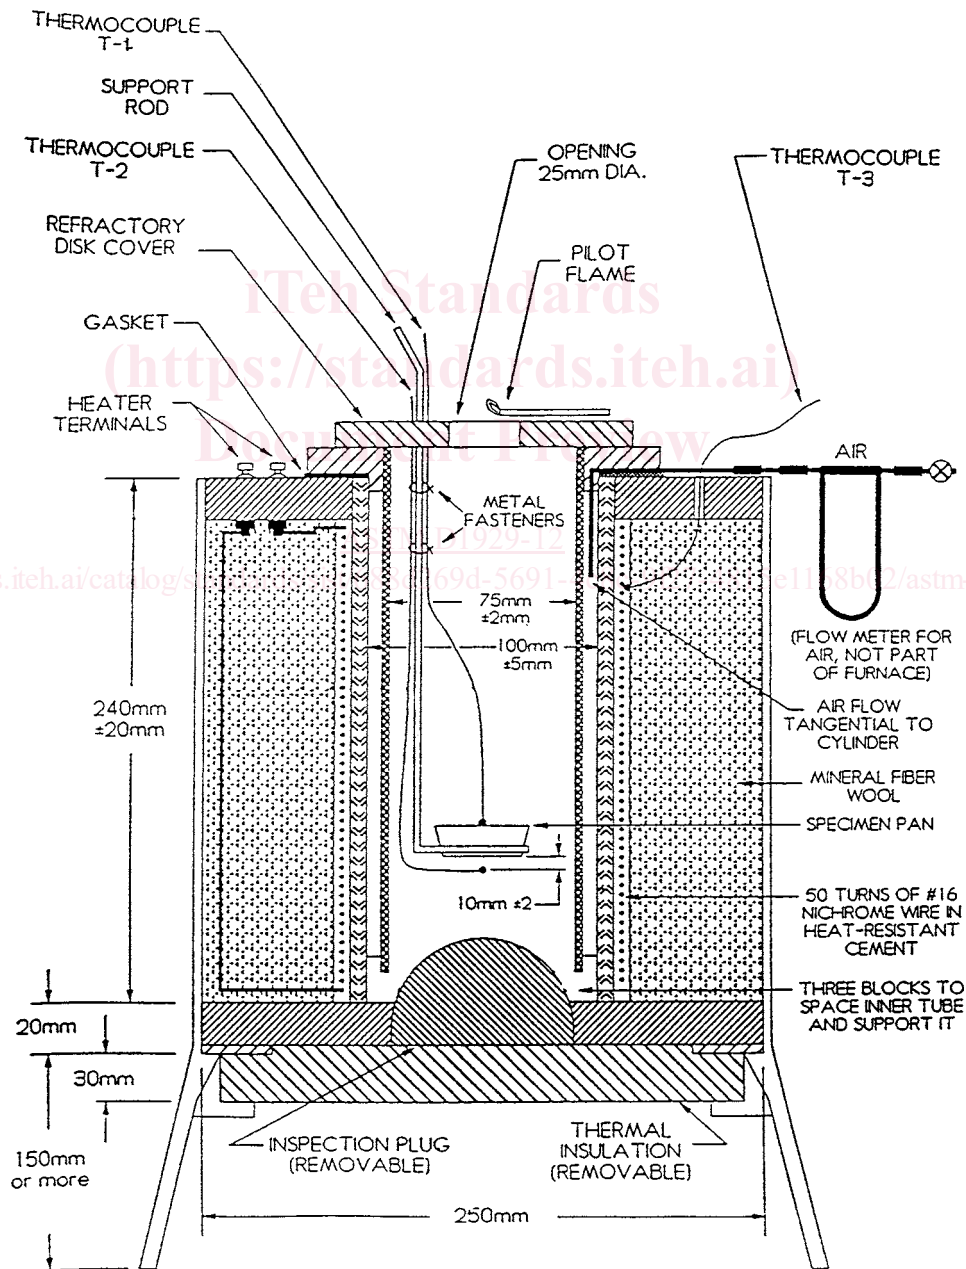


FIG. 1 Cross Section of Hot-Air Ignition Furnace