

# DRAFT INTERNATIONAL STANDARD

## ISO/DIS 16840-12

ISO/TC 173/SC 1

Secretariat: **SABS**

Voting begins on:  
**2021-02-08**

Voting terminates on:  
**2021-05-03**

---

---

## Wheelchair seating —

Part 12:

## Envelopment and immersion characterization of seat cushions using a dual semispherical indenter

ICS: 11.180.10

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

[ISO/DIS 16840-12](#)

<https://standards.iteh.ai/catalog/standards/sist/c7d417b1-e1c8-4e3d-94b2-c7a57dabd544/iso-dis-16840-12>

THIS DOCUMENT IS A DRAFT CIRCULATED FOR COMMENT AND APPROVAL. IT IS THEREFORE SUBJECT TO CHANGE AND MAY NOT BE REFERRED TO AS AN INTERNATIONAL STANDARD UNTIL PUBLISHED AS SUCH.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

This document is circulated as received from the committee secretariat.



Reference number  
ISO/DIS 16840-12:2021(E)

© ISO 2021

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO/DIS 16840-12  
<https://standards.iteh.ai/catalog/standards/sist/c7d417b1-e1c8-4e3d-94b2-c7a57dabd544/iso-dis-16840-12>



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2021

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

Page

<b>Foreword</b> .....	<b>iv</b>
<b>Introduction</b> .....	<b>v</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Indenter construction</b> .....	<b>2</b>
4.1 Materials.....	2
4.2 Tolerances and finishes.....	2
4.3 Indenter elements.....	2
4.3.1 Trochanter bar.....	2
4.3.2 Trochanter blocks.....	3
4.3.3 Semispherical indenter half.....	3
4.4 Indenter assembly.....	4
4.5 Sensor locations.....	5
4.5.1 General.....	5
4.5.2 Elevation a.....	6
4.5.3 Elevation b.....	6
4.5.4 Elevation c.....	6
4.5.5 Elevation d.....	6
<b>5 Instrumentation hardware</b> .....	<b>7</b>
5.1 Sensors.....	7
5.2 Timer.....	7
5.3 Loading equipment.....	7
5.4 Rigid board.....	7
<b>6 Preparation of test cushion</b> .....	<b>7</b>
6.1 Cushion set up.....	7
6.2 Preconditioning the cushion to the test environment.....	8
<b>7 Envelopment test method</b> .....	<b>8</b>
7.1 Rationale.....	8
7.2 Method.....	8
7.2.1 Setting the datum height for the indenter.....	8
7.2.2 Pre-conditioning the cushion.....	8
7.2.3 Seat cushion thickness measurement.....	8
7.2.4 Load application and data collection.....	9
7.3 Calculations.....	10
7.3.1 Envelopment.....	10
7.3.2 Immersion.....	11
<b>8 Test report</b> .....	<b>11</b>
<b>Annex A (informative) Estimate of measurement uncertainty</b> .....	<b>13</b>
<b>Bibliography</b> .....	<b>14</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 173, *Assistive products*, Subcommittee SC 01, *Wheelchairs*.

This second edition cancels and replaces the first edition (ISO/TS 16840-12:2015), which has been technically revised.

The main changes compared to the previous edition are as follows:

- are clarification of technical ambiguities, the removal of a gel cap to protect the pressure sensors, the removal of a superfluous Annex, and the addition of an Annex giving guidance on the estimation of uncertainty

A list of all parts in the ISO 16840 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

## Introduction

This document provides details of test equipment (an ‘indenter’), and a method, for the measurement of ‘performance’ of a wheelchair cushion intended to use immersion and envelopment to reduce local areas of pressure (by effectively supporting more tissue). Primary elements that represent the basic cushioning effect of a cushion are immersion and envelopment. Immersion into the cushion (the depth that a body penetrates into the surface) and the envelopment of the body (the intimacy of the cushion to the body) combine to define the potential cushioning performance of the cushion. Envelopment is maximized when the variation of forces across the weight bearing surface is minimized. The method as presented in this document is intended to quantify envelopment and immersion of the body by the cushion. Alternately, the test method and resulting data can provide an indication of other cushion construction and seating and positioning strategies, such as strategic pressure offloading.

Issues related to the use of devices that measure interface pressure between the body and a support surface (e.g. a pressure mapping system) have led to the use of an instrumented indenter, which has fewer sensors, but sensors which are high quality and exhibit repeatability and accuracy, and thus reliability.

In this test, the distribution of pressure across the surface of the indenter is evaluated with multiple indenter sizes and loads. The pressure sensors within the indenter are positioned at multiple elevations along the buttock form, to simulate and record the pressures experienced at the ischial tuberosities of the pelvis, the greater trochanters, and at positions along the curve of the buttocks between those anatomical markers. The review of the values at these various positions, and the variation, or lack of variation, in the readings, is an indication of the mechanics of the cushion’s interaction with the body and ability to envelop and protect the tissues.

**EXAMPLE** A fluid filled cushion with the ability to transfer material between cells may have the potential to distribute the load to maintain consistent interface pressure regardless of the depth at which the measurement is taken, as opposed to a foam or other homogeneous surface that behaves more like a spring, in that the greater the depth of immersion, the greater the interface pressure.

The accommodation of the cushion to the changes in indenter size and load are representative of the changes in size and mass of the occupant that can occur in the life of a user or between different users. The indenters are sized to represent changes in size and shape as a user of an approximately 410 mm cushion gains weight and the size of the buttocks increases. The overall width of the indenters stays the same, but the size of the semi spheres changes. The loads used in this document approximate to the 50<sup>th</sup> percentile user and are not intended to characterize envelopment or immersion under higher loading conditions, nor to assess the weight capacity of a cushion.

This standard describes test methods which may not be appropriate for all cushions, such as cushions using anisotropic materials, and therefore, the tester must determine which, if any, are appropriate for their cushion construction and use.

**iTeh STANDARD PREVIEW**  
**(standards.iteh.ai)**

ISO/DIS 16840-12

<https://standards.iteh.ai/catalog/standards/sist/c7d417b1-e1c8-4e3d-94b2-c7a57dabd544/iso-dis-16840-12>

# Wheelchair seating —

## Part 12:

# Envelopment and immersion characterization of seat cushions using a dual semispherical indenter

## 1 Scope

This document specifies apparatus, test methods, and disclosure requirements for characterization of wheelchair seat cushion immersion and envelopment properties using indenters instrumented with pressure sensors.

This document expands the characterization of products intended to manage tissue integrity (ISO 16840-2) and provides a standardized indenter for other wheelchair seating tests.

It does not provide information specific to cushion performance for a particular individual user, nor is it intended to characterize envelopment or immersion under higher loading conditions, nor to assess the weight capacity of a cushion.

This document includes a method that is specific to 220 mm and 255 mm indenters. Dimensions are provided for a 380 mm indenter to allow for extension of the method to larger patient simulation.

## 2 Normative references

[ISO/DIS 16840-12](#)

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1302, *Geometrical Product Specifications (GPS) — Indication of surface texture in technical product documentation*

ISO 16840-2, *Wheelchair seating — Part 2: Determination of physical and mechanical characteristics of seat cushions intended to manage tissue integrity*

## 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

### 3.1

#### **base point**

<indenter> lowest point on the curved surface of each of the two halves of the indenter

Note 1 to entry: The base points correspond with the ischial tuberosities on the human pelvis.

### 3.2

#### **elevation**

<indenter sensor> location of sensors relative to the base points of an indenter

### 3.3

#### **envelopment**

<cushion> ability to conform, around a shape

**3.4 immersion**

<cushion> depth from an uppermost plane to which a body penetrates

**3.5 offloading**

<clinical> reduction, removal, or transfer of pressure from one area of the body to another

EXAMPLE Reduction of pressure under the ischial tuberosities, but increased pressure on the thighs or other parts of the seated body.

**4 Indenter construction**

**4.1 Materials**

The indenter shall be constructed from hardwood or similar material that is sufficiently rigid so as not to deform when subjected to the forces required for simulating the application of a human body mass to surfaces. The indenter material shall be treated (if necessary) to minimize the effects of moisture, and shall not be adversely affected by normal laboratory testing conditions (0 °C to 35 °C; 25 % to 75 % relative humidity). Surface finish to be at least N7 (according to ISO 1302, approximate average surface roughness).

**4.2 Tolerances and finishes**

Unless otherwise stated, all dimensions in [Clause 4](#) shall be ± 0,5 mm and all edges and corners shall be finished with a minimum 5 mm radius. (standards.iteh.ai)


**4.3 Indenter elements**

ISO/DIS 16840-12

<https://standards.iteh.ai/catalog/standards/sist/c7d417b1-e1c8-4e3d-94b2-c7a57dabd544/iso-dis-16840-12>

**4.3.1 Trochanter bar**

A 375 mm x 50 mm x 20 mm bar with a series of openings as shown in Figure 1. These openings are for mounting the indenter halves and trochanter blocks as well as for routing of wires.

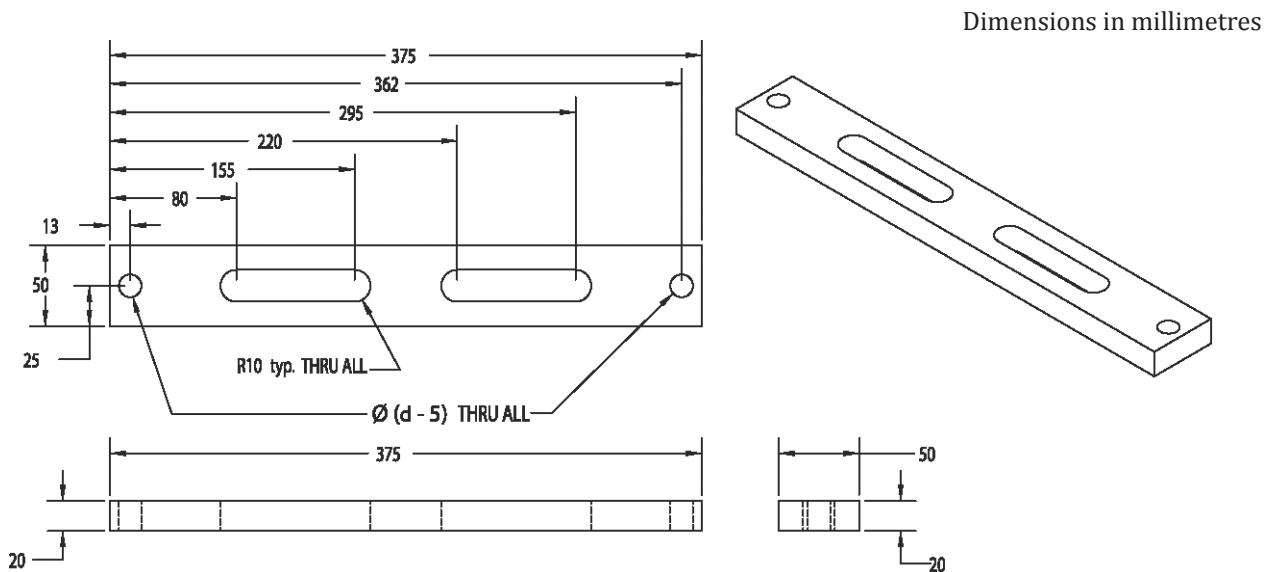

NOTE Dimension *d* is the diameter of the pressure sensor selected to meet requirements of [Clause 5.1](#). See [Clauses 4.1](#) and [4.2](#) for materials, tolerances, and finishes.

**Figure 1 — Trochanter bar construction**




### 4.3.2 Trochanter blocks

51 mm × 25 mm × 19 mm blocks as shown in [Figure 2](#), which emulate the trochanters. Each trochanter bar shall have two trochanter blocks which house the sensors.

NOTE Trochanter bar and blocks are not required on the 380 mm indenter.

Dimensions in millimetres

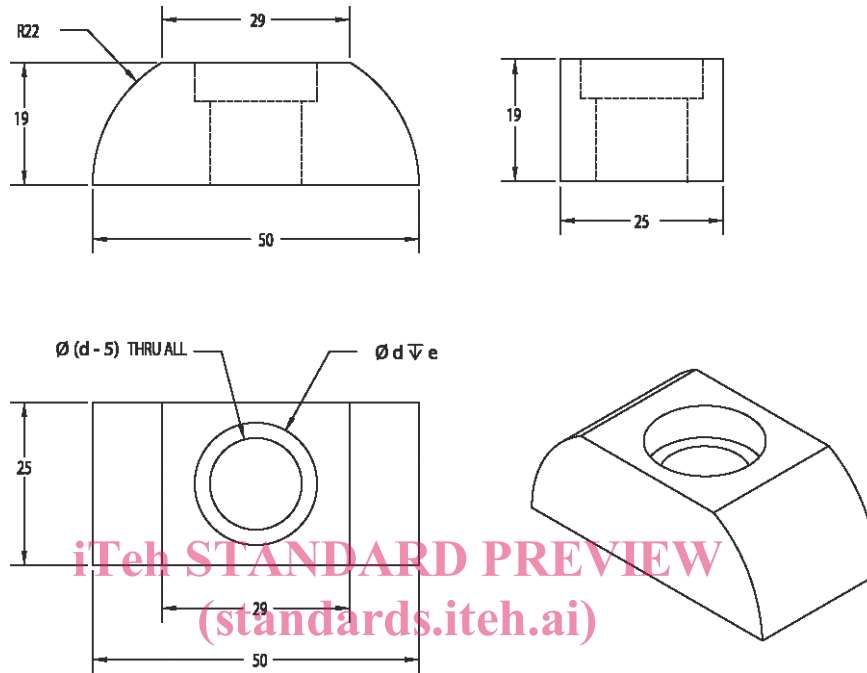


NOTE Dimension  $d$  is the diameter of the pressure sensor selected to meet requirements of [Clause 5.1](#). Sensor location depth should allow sensing surface to be flush with the indenter surface. See [Clauses 4.1](#) and [4.2](#) for materials, tolerances and finishes.

Figure 2 — Trochanter block construction

### 4.3.3 Semispherical indenter half

The semispherical indenter half is a portion of a sphere (see [Figure 3](#)). The sphere diameter defines the size of the indenter (e.g. a 220 mm indenter has two semispherical halves sectioned from a 220 mm diameter sphere) (see [Table 1](#)). Each half has eight sensor locations, as described in [Clause 4.5](#).

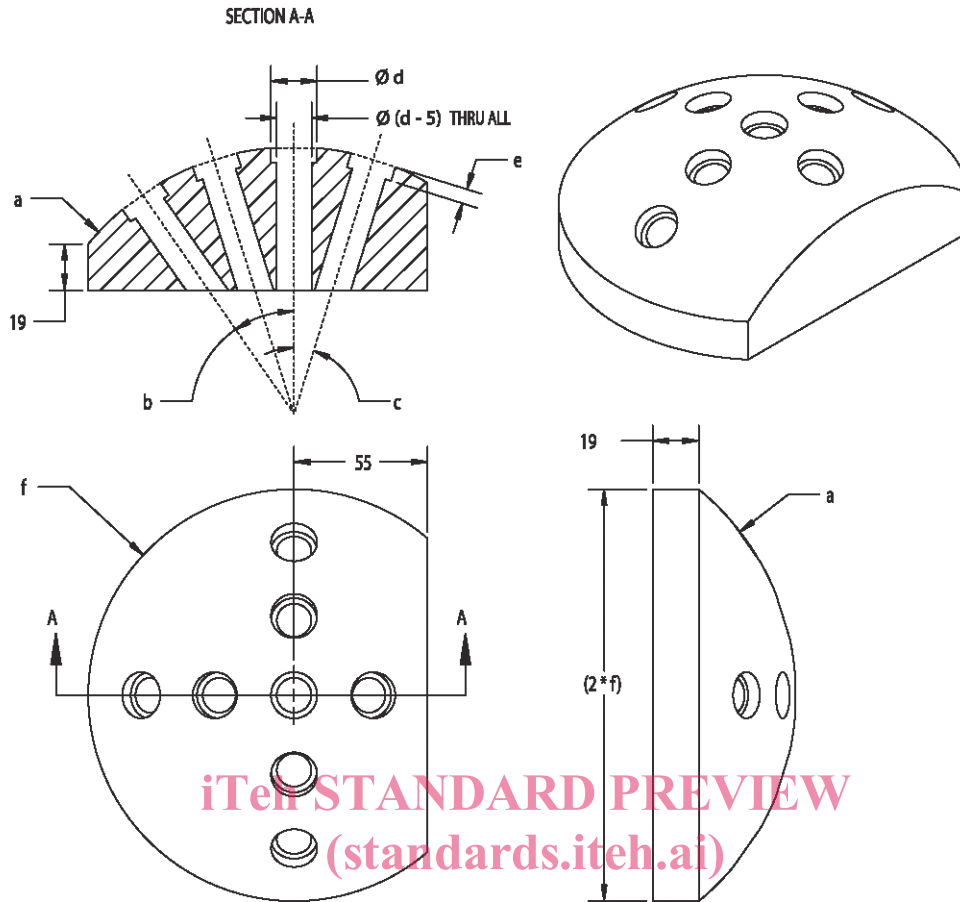

**Key**

- a radius of sphere
- b angle from centre sensor to farthest sensor (in all directions except cut direction)
- c angle from centre sensor to sensor adjacent to cut
- d diameter of hole for pressure sensor specified in [Clause 5.1](#)
- e depth of hole for pressure sensor specified in [Clause 5.1](#)
- f radius of disc

ISO/DIS 16840-12  
<https://standards.iteh.ai/catalog/standards/sist/c7d417b1-e1c8-4e3d-94b2-c7a57dabd544/iso-dis-16840-12>

NOTE See [Table 1](#) for dimensions. Sensor location depth should allow sensing surface to be flush with the indenter surface. See [Clauses 4.1](#) and [4.2](#) for materials, tolerances, and finishes.


**Figure 3 — Semispherical indenter half**

**Table 1 — Semispherical indenter dimensions**

INDENTER	a	b	c	f
220 mm	110 mm	35,0°	17,5°	85,0 mm
255 mm	127,5 mm	32,5°	16,0°	92,5 mm
380 mm	190 mm	26,5°	13,0°	128,5 mm


**4.4 Indenter assembly**

Assemble the indenter using appropriate fasteners that will maintain the structural integrity of the indenter in all aspects of testing. See [Figure 4](#) for assembly drawings for the 220 mm and 255 mm indenter and [Figure 5](#) for the 380 mm indenter.

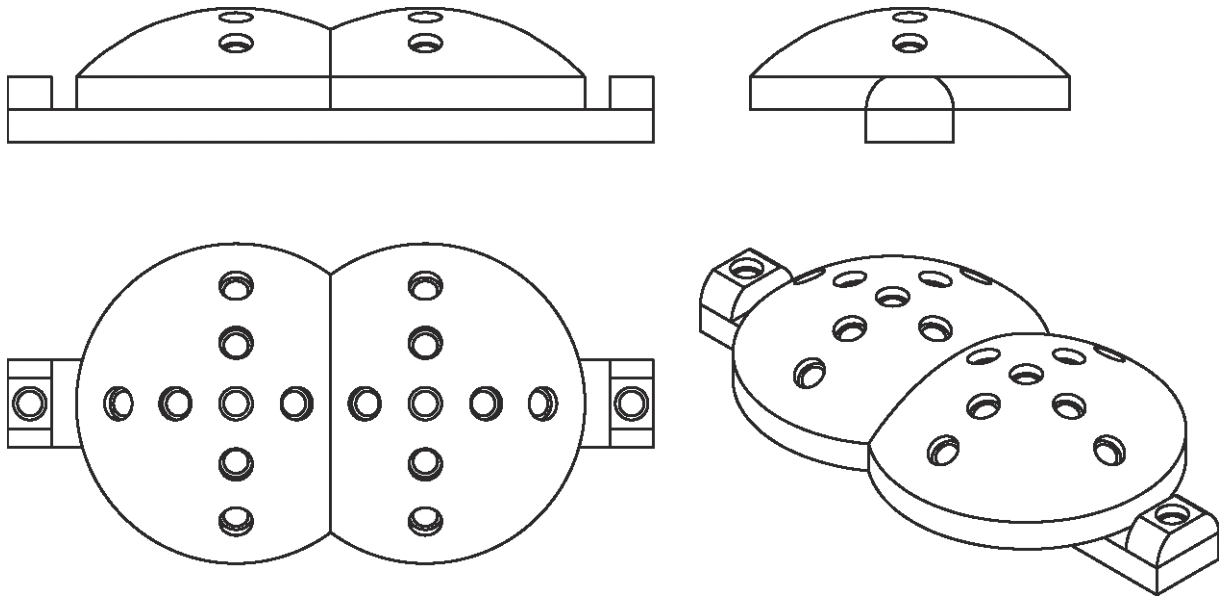

NOTE See [Clauses 4.1](#) and [4.2](#) for materials, tolerances, and finishes.

**Figure 4 — Indenter assembly for 220 mm and 255 mm indenters**

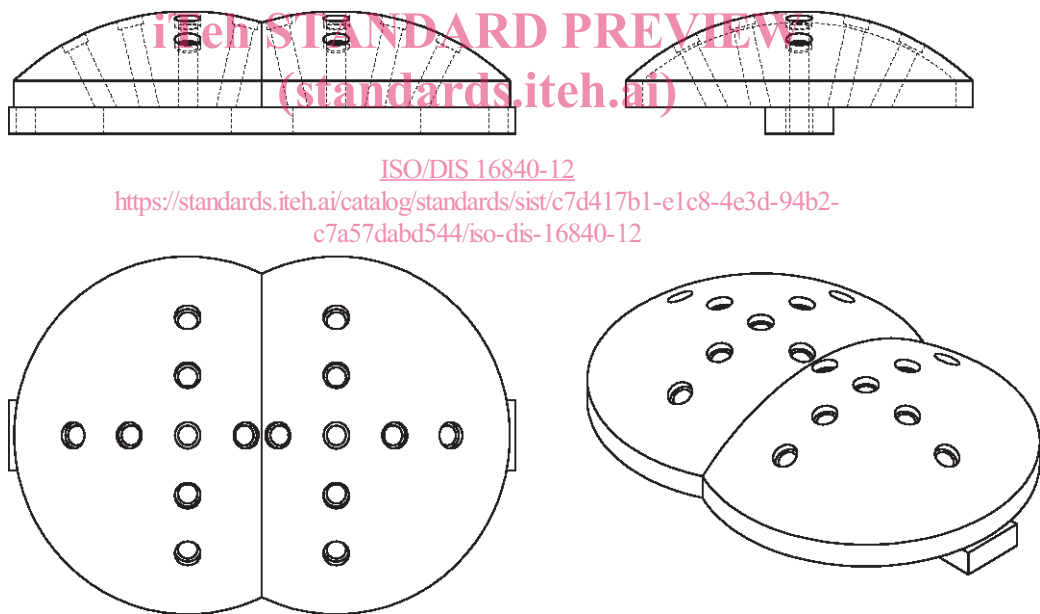

ISO/DIS 16840-12  
<https://standards.iteh.ai/catalog/standards/sist/c7d417b1-e1c8-4e3d-94b2-c7a57dabd544/iso-dis-16840-12>

NOTE See [Clauses 4.1](#) and [4.2](#) for materials, tolerances, and finishes.

**Figure 5 — Indenter assembly for 380 mm indenter**

## 4.5 Sensor locations

### 4.5.1 General

The following is a list of sensor locations and abbreviations. All sensors are symmetric about the midline of the instrumented indenter. For left and right sensor location configurations and elevations see [Figure 6](#) and [Figure 7](#).