



Designation: **D6342—08 D6342 – 12**

## Standard Practice for Polyurethane Raw Materials: Determining Hydroxyl Number of Polyols by Near Infrared (NIR) Spectroscopy<sup>1</sup>

This standard is issued under the fixed designation D6342; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

### 1. Scope\*

1.1 This standard covers a practice for the determination of hydroxyl numbers of polyols using NIR spectroscopy.

1.2 Definitions, terms, and calibration techniques are described. Procedures for selecting samples, and collecting and treating data for developing NIR calibrations are outlined. Criteria for building, evaluating, and validating the NIR calibration model are also described. Finally, the procedure for sample handling, data gathering and evaluation are described.

1.3 The implementation of this standard requires that the NIR spectrometer has been installed in compliance with the manufacturer's specifications.

1.4 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

NOTE 1—~~There~~ This standard is no equivalent or similar ISO standard: 15063.

### 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

**D883** Terminology Relating to Plastics

**D4274** Test Methods for Testing Polyurethane Raw Materials: Determination of Hydroxyl Numbers of Polyols

**D4855** Practice for Comparing Test Methods (Withdrawn 2008)<sup>3</sup>

**E131** Terminology Relating to Molecular Spectroscopy

**E168** Practices for General Techniques of Infrared Quantitative Analysis

**E222** Test Methods for Hydroxyl Groups Using Acetic Anhydride Acetylation

**E275** Practice for Describing and Measuring Performance of Ultraviolet and Visible Spectrophotometers

**E456** Terminology Relating to Quality and Statistics

**E1655** Practices for Infrared Multivariate Quantitative Analysis

**E1899** Test Method for Hydroxyl Groups Using Reaction with *p*-Toluenesulfonyl Isocyanate (TSI) and Potentiometric Titration with Tetrabutylammonium Hydroxide

2.2 *ISO Standard:*

**ISO 15063** Plastics—Polyols for use in the production of polyurethanes—Determination of hydroxyl number by NIR spectroscopy

### 3. Terminology

3.1 *Definitions*—Terminology used in this practice follows that defined in Terminology **D883**. For terminology related to molecular spectroscopy methods, refer to Terminology **E131**. For terms relating to multivariate analysis, refer to Practice **E1655**.

3.2 *Definitions of Terms Specific to This Standard:*

<sup>1</sup> This practice is under the jurisdiction of ASTM Committee **D20** on Plastics and is the direct responsibility of Subcommittee **D20.22** on Cellular Materials - Plastics and Elastomers.

Current edition approved March 1, 2008 Aug. 1, 2012. Published April 2008 September 2012. Originally approved in 1998. Last previous edition approved in 2003 2008 as **D6342 – 08** (2003). DOI: 10.1520/D6342-08.10.1520/D6342-12.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>3</sup> The last approved version of this historical standard is referenced on [www.astm.org](http://www.astm.org).

\*A Summary of Changes section appears at the end of this standard

3.2.1 *hydroxyl number*—the milligrams of potassium hydroxide equivalent to the hydroxyl content of 1 g of sample.

## 4. Summary of Practice

4.1 Multivariate mathematics is applied to correlate the NIR absorbance values for a set of calibration samples to the respective reference hydroxyl number for each sample. The resultant multivariate calibration model is then applied to the analysis of unknown samples to provide an estimate of their hydroxyl numbers.

4.2 Multilinear regression (MLR), principal components regression (PCR), and partial least squares regression (PLS) are the mathematical techniques used for the development of the calibration model.

4.3 Statistical tests are used to detect outliers during the development of the calibration model. Outliers can include high leverage samples and samples whose hydroxyl numbers are inconsistent with the model.

4.4 Validation of the calibration model is performed by using the model to analyze a set of validation samples. The hydroxyl number estimates for the validation set are statistically compared to the reference hydroxyl number for this set to test for agreement of the model with the reference method.

4.5 Statistical expressions are given for calculating the precision and bias of the NIR method relative to the reference method.

## 5. Significance and Use

### 5.1 General Utility:

5.1.1 It is necessary to know the hydroxyl number of polyols in order to formulate polyurethane systems.

5.1.2 This practice is suitable for research, quality control, specification testing, and process control.

### 5.2 Limitations:

5.2.1 Factors affecting the NIR spectra of the analyte polyols need to be determined before a calibration procedure is started. Chemical structure, interferences, any nonlinearities, the effect of temperature, and the interaction of the analyte with other sample components such as catalyst, water and other polyols needs to be understood in order to properly select samples that will model those effects which ~~can not~~ cannot be adequately controlled.

5.2.2 Calibrations are generally considered valid only for the specific NIR instrument used to generate the calibration. Using different instruments (even when made by the same manufacturer) for calibration and analysis can seriously affect the accuracy and precision of the measured hydroxyl number. Procedures used for transferring calibrations between instruments are problematic and are to be utilized with caution following the guidelines in Section 16. These procedures generally require a completely new validation and statistical analysis of errors on the new instrument.

5.2.3 The analytical results are statistically valid only for the range of hydroxyl numbers used in the calibration. Extrapolation to lower or higher hydroxyl values can increase the errors and degrade precision. Likewise, the analytical results are only valid for the same chemical composition as used for the calibration set. A significant change in composition or contaminants can also affect the results. Outlier detection, as discussed in Practices E1655, is a tool that can be used to detect the possibility of problems such as those mentioned above.

## 6. Instrumentation

6.1 *Introduction*—A complete description of all applicable types of NIR instrumentation is beyond the scope of this standard. Only a general outline is given here. A diagram of a typical NIR spectrometer is shown in Fig. 1.

6.2 *Light Source and Detector*—Tungsten-halogen lamps with quartz envelopes usually serve as the energy sources for NIR instruments. Most of the detectors used for NIR are solid-state semiconductors. PbS, PbSe, and InGaAs detectors are most commonly used.

6.3 *Light Dispersion*—Spectrophotometers can be classified based on the procedure by which the instrument accomplishes wavelength selection.

6.3.1 *Monochromator Instrument*—Grating monochromator instruments, often called “dispersive” instruments, are commonly used in the laboratory and for process applications. In a holographic grating system, the grating is rotated so that only a narrow band of wavelengths is transmitted to a single detector at a given time.

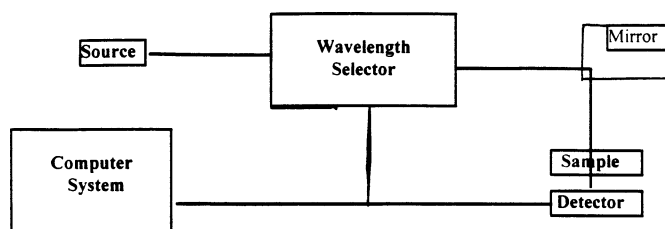


FIG. 1 Schematic of a Near-IR System