



Designation: E1672-06 Designation: E1672 - 12

Standard Guide for Computed Tomography (CT) System Selection¹

This standard is issued under the fixed designation E1672; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

This standard has been approved for use by agencies of the Department of Defense.

1. Scope Scope*

1.1 This guide covers guidelines for translating application requirements into computed tomography (CT) system requirements/specifications and establishes a common terminology to guide both purchaser and supplier in the CT system selection process. This guide is applicable to the purchaser of both CT systems and scan services. Computed tomography systems are complex instruments, consisting of many components that must correctly interact in order to yield images that repeatedly reproduce satisfactory examination results. Computed tomography system purchasers are generally concerned with application requirements. Computed tomography system suppliers are generally concerned with the system component selection to meet the purchaser's performance requirements. This guide is not intended to be limiting or restrictive, but rather to address the relationships between application requirements and performance specifications that must be understood and considered for proper CT system selection.

1.2 Computed tomography (CT) may be used for new applications or in place of film radiography, provided that the capability to disclose physical features or indications that form the acceptance/rejection criteria is fully documented and available for review.

1.3 Computed tomography (CT) systems use a set of transmission measurements made along a set of paths projected through the object from many different directions. Each of the transmission measurements within these views is digitized and stored in a computer, where they are subsequently conditioned (for example, normalized and corrected) and reconstructed by one of a variety of techniques. An in-depth treatment of CT principles is given in Guide

1.2 Computed tomography (CT) may be used for new applications or in place of radiography or radioscopy, provided that the capability to disclose physical features or indications that form the acceptance/rejection criteria is fully documented and available for review. In general, CT has lower spatial resolution than film radiography and is of comparable spatial resolution with digital radiography or radioscopy unless magnification is used. Magnification can be used in CT or radiography/radioscopy to increase spatial resolution but concurrently with loss of field of view.

1.3 Computed tomography (CT) systems use a set of transmission measurements made along a set of paths projected through the object from many different directions. Each of the transmission measurements within these views is digitized and stored in a computer, where they are subsequently conditioned (for example, normalized and corrected) and reconstructed, typically into slices of the object normal to the set of projection paths by one of a variety of techniques. If many slices are reconstructed, a three dimensional representation of the object is obtained. An in-depth treatment of CT principles is given in Guide E1441.

1.4 Computed tomography (CT), as with conventional radiography and radioscopy examinations, is broadly applicable to any material or object through which a beam of penetrating radiation may be passed and detected, including metals, plastics, ceramics, metallic/nonmetallic composite material and assemblies. The principal advantage of CT is that it provides has the potential to provide densitometric (that is, radiological density and geometry) images of thin cross sections through an object. In many newer systems the cross-sections are now combined into 3D data volumes for additional interpretation. Because of the absence of structural superposition, images are may be much easier to interpret than conventional radiological images. The new purchaser can quickly learn to read CT data because images correspond more closely to the way the human mind visualizes 3D structures than conventional projection radiology. Further, because CT images are digital, the images may be enhanced, analyzed, compressed, archived, input as data into performance calculations, compared with digital data from other nondestructive evaluation modalities, or transmitted to other locations for remote viewing. 3D data sets can be rendered by computer graphics into solid models. The solid models can be sliced or segmented to reveal 3D internal information or output as CAD files. While many of the details are generic in nature, this guide implicitly assumes the use of penetrating radiation, specifically X rays and gamma rays.

1.5 Units—The values stated in SI units are to be regarded as standard. The values given in parentheses are mathematical

¹ This guide is under the jurisdiction of ASTM Committee E07 on Nondestructive Testing and is the direct responsibility of Subcommittee E07.01 on Radiology (X and Gamma) Method.

Current edition approved Dec. 1, 2006. Published January 2007. Originally approved in 1995. Last previous edition approved in 2001 as E1672-95(2001)¹. DOI: 10.1520/E1672-06.

Current edition approved June 15, 2012. Published September 2012. Originally approved in 1995. Last previous edition approved in 2006 as E1672-06. DOI: 10.1520/E1672-12.

*A Summary of Changes section appears at the end of this standard.

conversions to inch-pound units that are provided for information only and are not considered standard.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:²

E1316 [Terminology for Nondestructive Examinations](#)

E1441 [Guide for Computed Tomography \(CT\) Imaging](#)

E1570 [Practice for Computed Tomographic \(CT\) Examination](#) ~~Practice for Computed Tomographic (CT) Examination~~

E2339 [Practice for Digital Imaging and Communication in Nondestructive Evaluation \(DICONDE\)](#)

E2767 [Practice for Digital Imaging and Communication in Nondestructive Evaluation \(DICONDE\) for X-ray Computed Tomography \(CT\) Test Methods](#)

3. Terminology

3.1 *Definitions*—For definitions of terms used in this guide, refer to Terminology E1316 and Guide E1441, Appendix X1.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *purchaser*—purchaser or customer of CT system or scan service.

3.2.2 *scan service*—use of a CT system, on a contract basis, for a specific examination application. A scan service acquisition requires the matching of a specific examination application to an existing CT machine, resulting in the procurement of CT system time to perform the examination. Results of scan service are contractually determined but typically include some, all, or more than the following: meetings, reports, images, pictures, and data.

3.2.3 *subsystem*—one or more system components integrated together that make up a functional entity.

3.2.4 *supplier*—suppliers/owners/builders of CT systems.

3.2.5 *system component*—generic term for a unit of equipment or hardware on the system.

3.2.6 *throughput*—number of CT scans performed in a given time frame.

4. Summary of Guide

4.1 This guide provides guidelines for the translation of examination requirements to system components and specifications. Understanding the CT purchaser's perspective as well as the CT equipment supplier's perspective is critical to the successful acquisition of new CT hardware or implementation, or both, of a specific application on existing equipment. An understanding of the performance capabilities of the system components making up the CT system is needed in order for a CT system purchaser to prepare a CT system specification. A specification is required for acquisition of either CT system hardware or scan services for a specific examination application.

4.2 Section 7 identifies typical purchaser's examination requirements that must be met. These purchaser requirements factor into the system design, since the system components that are selected for the CT system will have to meet the purchaser's requirements. Some of the purchaser's requirements are: the ability to support the object under examination, that is, size and weight; detection capability for size of defects and flaws, or both, (spatial resolution and contrast discrimination); dimensioning precision; artifact level; throughput; ease of use; archival procedures. Section 7 also describes the trade-offs between the CT performance as required by the purchaser and the choice of system components and subsystems.

4.3 Section 8 covers some management cost considerations in CT system procurements.

4.4 Section 9 provides some recommendations for the procurement of CT systems.

5. Significance and Use

5.1 This guide will aid the purchaser in generating a CT system specification. This guide covers the conversion of purchaser's requirements to system components that must occur for a useful CT system specification to be prepared.

5.2 Additional information can be gained in discussions with potential suppliers or with independent consultants.

5.3 This guide is applicable to purchasers seeking scan services.

5.4 This guide is applicable to purchasers needing to procure a CT system for a specific examination application.

6. Basis of Application

6.1 The following items should be agreed upon by the purchaser and supplier.

6.1.1 *Requirements*—General system requirements are covered in Section 7.

7. Subsystems Capabilities and Limitations

7.1 This section describes how various examination requirements affect the CT system components and subsystems. Trade-offs

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

between requirements and hardware are cited. Table 1 is a summary of these issues. Many different CT system configurations are possible due to the wide range of system components available for integration into a single system. It is important to understand the capability and limitations of utilizing one system component over another as well as its role in the overall subsystem. Fig. 1 is a functional block diagram for a generic CT system.

7.1.1 Pencil-Beam, Fan-Beam and Cone-Beam Type Systems:

7.1.1.1 Pencil Beam Systems—The x-ray beam is collimated to a pencil and the effective pixel size becomes the size of the beam on the detector area. The beam is translated over the object and the object rotated after each pass of the beam over the object or the beam and detector are translated and rotated around the object to build up linear slice profiles. If a three dimensional data set is desired the object or beam/detector must elevate so that multiple slices are generated. The advantage of this method is detector simplicity and scatter rejection with the primary disadvantage being long scan times.

7.1.1.2 Fan-Beam Systems—The x-ray beam is collimated to a fan and detected by a linear detector array that usually has a collimator aperture. The pixel size is defined by the width of the fan-beam on the detector height (vertically) and by the detector element pitch (horizontally). Linear profiles are captured as the object or beam/detector rotates. If three dimensional data is desired the object or beam/detector must elevate to capture multiple slices. The advantage of this method is faster scan times than pencil-beam systems and some scatter rejection with the primary disadvantage being long scan times for 3D data.

7.1.1.3 Cone-Beam Systems—The x-ray beam is usually collimated to the entire or a selected portion of the active area of a two dimensional detector array and full 2D images are captured as the object or beam/detector rotates. In this manner multiple slices are generated without needing to elevate. The primary advantage of this technique is speed or acquiring 3D data, with the primary disadvantage being increased scatter due to larger field of view.

7.2 Object, Size and Weight—The most basic consideration for selecting a CT system is the examination object’s physical dimensions and characteristics, such as size, weight, and material. The physical dimensions, weight, and attenuation of the object dictate the size of the mechanical subsystem that handles the examination object and the type of radiation source and detectors, or both, needed. To select a system for scan services, the issues of CT system size, object size and weight, and radiation energy must be addressed first. Considerations like detectability and throughput cannot be addressed until these have been satisfactorily resolved. Price-performance tradeoffs must be examined to guard against needless costs.

7.2.1 The maximum height and diameter of an object that can be examined on a CT system defines the equipment examination envelope. The weight of the object and any associated fixturing must be within the manipulation system capability. For example, a very different mechanical sub-system will be required to support and accurately move a large, heavy object than to move a small, light object. Similarly, the logistics and fixturing for handling a large number of similar items will be a much different problem than for handling a one-of-a-kind item.

7.2.1 The maximum height and diameter of an object that can be examined on a CT system defines the equipment examination envelope. Data must be captured over the entire width of the object for each view. If the projected x-ray beam through the object does not provide complete coverage, the object or beam/detector must translate. Some specialized algorithms may allow the reduction of this requirement but detectability and scan time may be affected. The weight of the object and any associated fixturing

<https://standards.iteh.ai/catalog/standards/sist/32660a55-97bd-4a2f-be35-6ee82b3f132b/astm-e1672-12>

TABLE 1 Computed Tomography (CT) System Examination Requirements and Their Major Ramifications

Requirement	Components/Subsystems Affected	Reference
Object, size and weight	Mechanical handling equipment	7.2
Object radiation penetrability	Dynamic range	7.3
Detectability	Radiation source	7.3.1
		7.4
Spatial resolution	Detector size/aperture	7.4.1.1
	Source size/source spot size	7.4.1.2
	Mechanical handling equipment	7.4.1.5
Contrast discrimination	Strength/energy of radiation source	7.4.2
	Detector size/source spot size	7.4.2.1
Artifact level	Mechanical handling equipment	7.4.3
Throughput/speed of CT process		7.5
Scan time	(Spatial resolution)	7.5.1
	(Contrast discrimination)	
Image matrix size (number of pixels in image)	Number/configuration of detectors	7.5.2
	Amount of data acquired	
Slice thickness range	Computer/hardware resources	
	Detector configuration/collimators	7.5.3
Operator interface	System dynamic range	
		7.6
	Operator console	7.6.1
Ease of use	Computer resources	7.6.2
		7.6.3
Trade-offs		7.6.4

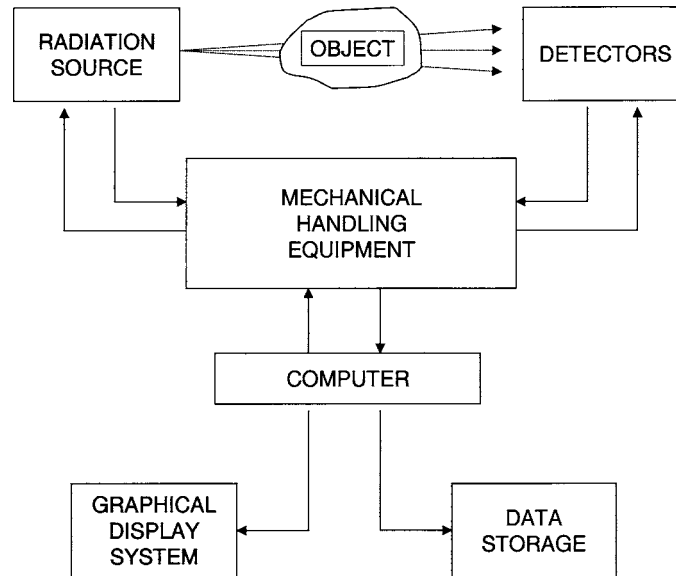


FIG. 1 Functional Block Diagram for a Generic CT System

must be within the manipulation system capability. For example, a very different mechanical sub-system will be required to support and accurately move a large, heavy object than to move a small, light object. Similarly, the logistics and fixturing for handling a large number of similar items will be a much different problem than for handling a one-of-a-kind item.

7.2.2 Two Most Common Types of Scan Motion Geometries:—Both geometries are applicable to 2D fan beam or 3D cone beam systems.

7.2.2.1 Translate-Rotate Motion—The object or detector is translated in a direction perpendicular to the direction and parallel to the plane of the X-ray beam. Full data sets are obtained by rotating the article between translations by the fan angle of the beam and again translating the object until a minimum of 180° of data have been acquired. The advantage of this design is simplicity, good view-to-view detector matching, flexibility in the choice of scan parameters, and ability to accommodate a wide range of different object sizes, including objects too big to be subtended by the X-ray fan. The disadvantage is longer scan time. Reconstruction software must correctly account for fan/cone beam effects which can be complicated by translation of the object.

7.2.2.2 Rotate-Only Motion—The object remains stationary and the source and detector system is rotated around it. A complete view is collected by the detector array during each sampling interval. A rotate-only scan has lower motion overhead than a translate-rotate scan, and is attractive for industrial applications where the object to be examined fits within the fan beam, and scan speed is important. Irrespective of whether the sample translates and rotates, or both, or the source/detector system rotates, the principles of CT are the same.—The object remains stationary and the source and detector system is rotated around it or the object rotates and the source and detector remain stationary. A complete view is generally collected by the detector array during each sampling interval. A rotate-only scan has lower motion overhead than a translate-rotate scan, and is attractive for industrial applications where the object to be examined fits within the fan beam, and scan speed is important. Irrespective of whether the sample translates and rotates, or both, or the source/detector system rotates, the principles of CT are the same. In 2D fan beam type systems, the sample/object may also be elevated through the fan beam in order to build up a three dimensional stack of cross-sectional views. In a cone beam type system, the rows of the detector array provide the third dimension. The sample/object may need to be elevated or translated in order to provide complete coverage if the sample/object is larger than the cone beam (the projected area of the sample/object on the detector array area.) For some applications a rotate/translate combination, or helical, scan may be appropriate.

7.2.3 The purchaser of CT equipment should be aware that important cost trade-offs may exist. For instance, the cost of a mechanical subsystem with translate, rotate, and elevate functions incorporated in one integrally constructed piece of hardware is relatively cost invariant for vertical motions up to some limit, but increases drastically above that point. The casual specification of an elevation could have severe cost implications; whereas the simple expediency of turning the object over could effectively extend the examination envelope with no cost impact. Similarly, the specification of a large field of view could drive system size and cost soaring; whereas the application of prior information or limited angle reconstruction techniques, or both, could enable the examination with a much smaller scanner.

7.2.4 Automatic material handling equipment is an option that can be acquired with a CT system for mounting and removing objects. The advantages are lower overhead and greater throughput. The main disadvantages are added costs and complexity to the system design.

7.3 Object Radiation Penetrability—Next to examination envelope and weight, the most basic consideration is radiation penetrability. Object penetrability determines the minimum effective energy and intensity for the radiation source. As in any radiological situation, penetrability is a function of object material, density and morphology (shape and features/geometry). The

rules for selecting CT source energy are approximately the same as those for conventional radiography, with the understanding that for CT, the incident radiation must be able to penetrate the maximum absorption path length through the object in the plane of the scan. The lowest signal value should be larger than the root-mean-square (RMS) of the electronic noise. The required flux is determined by how many photons are needed for statistical considerations. The spot size is determined by the spatial resolution and specimen geometry requirements.

7.3.1 *X-ray Sources*—Electrical X-ray generators offer a wider selection in peak energy and intensity and have the added safety feature of discontinued radiation production when switched off. The disadvantage is that the polychromaticity of the *Bremsstrahlung* energy spectrum causes artifacts such as cupping (the anomalous decreasing attenuation toward the center of a homogeneous object) in the image if uncorrected. Filtering of the x-ray beam can “Harden” the x-ray spectrum by reducing the amount of lower energies which can help reduce artifacts. Harder beam spectrum results in lower image contrast and may need for higher primary beam exposure dose, therefore, selection of the correct filtering is very important. X-ray tubes and linear accelerators (linacs) are typically several orders of magnitude more intense than isotope sources. However, X-ray generators have the disadvantage that they are inherently less stable than isotope sources. X rays produced from electrical radiation generators have source spot sizes ranging from a few millimetres down to a few micrometres. Reducing the source spot size reduces geometric unsharpness, thereby enhancing detail sensitivity. However, the basic spatial resolution (SRb) of the detector must also be able to support this increased spatial resolution. Smaller source spots permit higher spatial resolution but at the expense of reduced X-ray beam intensity. Reduced X-ray beam intensity implies that only smaller longer scan times or less dense objects can be inspected. inspection of smaller or less dense objects. Also to keep in mind, unlike radiography, CT can require extended, continuous usage of the X-ray generator. Therefore, an increased cooling capacity of the X-ray generator should be considered in the design and purchase, ~~or both~~, in anticipation of the extended usage requirements.

7.3.2 *Radioisotope Sources*—A radioisotope source can have the advantages of small physical size, portability, low-power requirements, simplicity, discrete spectral lines, and stability of output. The disadvantages are limited intensity per unit area, limited peak energy, and increased regulatory concerns.

7.3.3 *Synchrotron Radiation (SR) Sources*—Synchrotron radiation (SR) sources with special equipment (like monochromators) produce very intense, naturally collimated, narrow bandwidth, tunable radiation. Thus, CT systems using SR sources can employ essentially monochromatic radiation. With present technology, however, practical SR energies are restricted to less than about 20 to 30 keV. Since any CT system is limited to the examination of samples with radio-opacities consistent with the penetrating power of the X rays or gamma rays employed, SR systems can, in general, image only small (1- to 5-mm) objects.

7.3.4 Oftentimes, filters and compensators are used to tune the source to the desired output. The use of filters and compensators will reduce the full capability of the source, causing additional limitations to source output.—Synchrotron radiation (SR) sources with special equipment (like monochromators) produce very intense, naturally collimated, narrow bandwidth, tunable radiation. Thus, CT systems using SR sources can employ essentially monochromatic radiation. With present technology, however, practical SR energies are restricted to less than about 20 to 30 keV. Since any CT system is limited to the examination of samples with radio-opacities consistent with the penetrating power of the X rays or gamma rays employed, monochromatic SR systems can, in general, image only small (1- to 5-mm) low density objects. Some synchrotron sources also have a polychromatic, or white, beam line available allowing CT of higher density materials. It should also be noted that synchrotrons produce a wide flat beam, typically several centimeters wide by a few hundred microns tall. This means an object is typically translated to obtain a full 3D. In addition to the above consideration a synchrotron beams are virtually parallel which means resolution depends primarily on the detector's effective pixel size. For this reason high end cameras and scintillators are typically employed.

7.3.4 *Filters*—Oftentimes, filters and compensators are used to tune the source to the desired output. The use of filters and compensators will reduce the full capability of the source, causing additional limitations to source output.

7.4 *Detectability*—Once the basic considerations of object size, weight, and radiation penetrability have been addressed, the specific examination requirements are handled. The most important is the capability of the CT system to image the characteristics of concern in the object. This is a detectability issue. Detectability is an all-encompassing term that includes elements of spatial resolution, contrast discrimination, and artifacts. Spatial resolution characterizes how faithfully the CT system reproduces the features of the examination specimen in an image. Contrast discrimination characterizes the amount of random noise in the CT image and the ability to detect features within noise, that is, the signal to noise ratio for a given feature of interest. The former quantifies our knowledge of an object, the latter our uncertainty. Together, they form a complementary pair of variables that fully characterize any imaging system. Artifacts are reproducible features in an image that are not related to actual features in the object. The purchaser is normally interested in detecting geometrical (dimensional) and material (density, porosity, inclusions, etc.) anomalies. From experience, allowable variations are generally known and codified. They usually take the form of simple declarative statements: For example: Critical dimensions must be accurate to $\pm 25 \mu\text{m}$ (0.001 in.); Void diameters must be less than 1 mm (0.040 in.); Porosity must represent less than 1 % missing volume; Density variations over 1 cm^2 (0.40 in.²) must be less than 1 %; etc. These so-called application requirements are often explicitly known. The system component engineer must determine the spatial resolution and contrast discrimination needed to obtain the specified dimensional accuracy and defect sensitivity. This in turn sets upper limits on the amount or type, or both, of artifacts that can be tolerated. Making this connection between specifications and performance requirements is generally a difficult task that is best solved collaboratively between purchaser and supplier.

7.4.1 *Spatial Resolution*—All imaging systems, CT included, are limited in their ability to reproduce object morphology. Sometimes features can be detected but not accurately measured. That is, an infinitely small, infinitely dense point in the object will be imaged not as a point, but as a spot—possibly a very small spot, but a spot of finite size nonetheless. Hence, the image of a real object will exhibit a certain amount of unsharpness. Computed tomography (CT) unsharpness (blurred edges). CT spatial resolution is a measure of this unsharpness and obeys much the same rules as any radiological imaging modality: it is limited by the effective in-plane size of the detectors (pixels), the in-plane size of the source spot, and the relative position of the specimen with respect to the source and detector. Other factors, such as sampling, motion uncertainty, reconstruction matrix size, image display matrix, and reconstruction algorithms, can degrade the inherent spatial resolution.

7.4.1.1 *Radiation Detection*—The detection system converts the transmitted radiation into an electronic signal. The detector element is typically a scintillation detector that is optically coupled to a photo-conversion device such as a photodiode or photomultiplier tube. Alternatively, some systems use other types of detectors. For fan-beam type systems, the in-plane detector width is determined in part by the spatial resolution requirement. This detector width is either designed in the system or, for variable aperture systems, can be set by some kind of shielding aperture plates that define the detector's field of view. The detection system may consist of a single sensing element, an area array of sensing elements, or a linear array of sensing elements. The more detectors used, the faster the required scan data can be collected; but there are important trade-offs to be considered.

(1) A single detector provides the least efficient method of collecting data but entails minimal complexity, eliminates concerns of scatter between elements and differences in detector response, and allows an arbitrary degree of collimation and shielding. A single detector provides the least efficient method of collecting data but entails minimal complexity, eliminates concerns of scatter between elements, differences in detector response, and allows an arbitrary degree of collimation and shielding. Translation motion is required for two dimensional reconstructions and elevate motion is required to create three dimensional reconstructions.

(2) An area detector provides the most efficient method of collecting data but entails the transfer and storage of large amounts of information, forces trade-offs between scatter, elements, and detector efficiency, and creates serious collimation and shielding challenges. An area detector provides the most efficient method of collecting data but entails the transfer and storage of large amounts of information, forces trade-offs between scatter, elements, and detector efficiency, and creates serious collimation and shielding challenges. However, using cone beam reconstruction algorithms three dimensional renderings of the object can be made. Guide E2736 contains information about area digital detector arrays.

(3) Linear arrays have performance characteristics intermediate between these two extremes, for example, reasonable scan times at moderate complexity, acceptable scatter between elements, and differences in detector response. Linear arrays have a flexible architecture that typically accommodates good collimation and shielding. Linear arrays have performance characteristics intermediate between these two extremes, for example, reasonable scan times at moderate complexity, acceptable scatter between elements, and differences in detector response. Linear arrays have a flexible architecture that typically accommodates good collimation and shielding but require elevate motion for three dimensional reconstructions. In some cases several linear areas are combined to allow faster scans while keeping some of the collimation benefits.

(4) An important aspect of the detection system is the electronics system used to convert the analog signal received to a digital stream for processing. The front-end analog electronics amplify the detector signal to a magnitude that can be digitized. Fast systems demand good fidelity of the amplified signal. What makes the task especially demanding is that many signals, differing by several orders of magnitude, are frequently multiplexed on the same line in rapid succession; intersignal amplification rates are measured in microseconds. The analog-to-digital (A/D) conversion is performed as close to the analog amplification chain as possible. The accuracy requirement of the A/D must be consistent with the statistical limitations of the largest and the smallest detectable signals.

7.4.1.2 *Source Spot Size*—The source spot is the source region from which X rays or gamma rays emanate. In an electrical radiation generator, like an X-ray tube or linear accelerator, it is the area where the electrons strike the target. In an isotopic source, it is the area from which the radiation effectively emerges. The size and shape of the source spot is an important determinant of the aperture function (see ASTM source focal spot standards). For instance, source spots in linear accelerators are typically shaped as Gaussian distributions; whereas source spots in X-ray tubes are often double-peaked. Source spots associated with isotopic sources can be either more or less complex. Since source spots do not generally have sharp edges—or even symmetric shapes, it is common practice to define an effective size for convenience. The actual intensity distribution is important information, but is too complex to be readily useful. Consequently, reported source spot sizes are a function of the definition and method used to measure them. For example, the average radius of the region from which 99 % of the emissions emerge will be much larger than the standard deviation of the intensity distribution. In other words, source spot characteristics can be quantified in different ways. For this reason, comparisons between sources, especially those provided by different suppliers, are difficult to make. Another source selection factor to consider is stability. In selecting an electrical source, appreciate that spot position can wander over time, and changes in accelerating potential can occur.

7.4.1.3 Often, the in-plane source spot size and the in-plane detector width can be adjusted over a limited range of options, allowing spatial resolution to be engineered somewhat. Spatial resolution is a combination of geometrical and detector factors with the geometrical contribution dependent on focal spot size. In general, the smaller the source spot or detector size, or both, the better the spatial resolution. Since spatial resolution limits dimensional accuracy and resolving power (that is, the ability to distinguish two nearby point objects as separate entities), pressure exists it is desired to select the smallest possible source spot and detector