

DRAFT INTERNATIONAL STANDARD

ISO/DIS 17328

ISO/TC 172/SC 3

Secretariat: JISC

Voting begins on:
2021-01-08

Voting terminates on:
2021-04-02

Optics and photonics — Optical materials and components — Test method for refractive index of infrared optical materials

*Optique et photonique — Matériaux et composants optiques — Méthode d'essai de l'indice de réfraction
des matériaux optiques infrarouges*

ICS: 37.020

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO/DIS 17328](#)

<https://standards.iteh.ai/catalog/standards/sist/3dfaebae-345a-48c5-8b93-970b7dbeb23e/iso-dis-17328>

THIS DOCUMENT IS A DRAFT CIRCULATED FOR COMMENT AND APPROVAL. IT IS THEREFORE SUBJECT TO CHANGE AND MAY NOT BE REFERRED TO AS AN INTERNATIONAL STANDARD UNTIL PUBLISHED AS SUCH.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

This document is circulated as received from the committee secretariat.



Reference number
ISO/DIS 17328:2021(E)

© ISO 2021

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO/DIS 17328

<https://standards.iteh.ai/catalog/standards/sist/3dfaebae-345a-48c5-8b93-970b7dbeb23e/iso-dis-17328>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2021

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Method for measuring	2
4.1 General	2
4.2 Principle	2
4.3 Apparatus and procedure for measurement	3
4.4 Wavelength of light beam for measurement	3
5 Specimens	4
5.1 The shape and dimensions of the specimen prism	4
5.2 Surface accuracy	4
6 Test report	4
Annex A (informative) Apparatus for measurement	6
Annex B (informative) Analysis of errors	13
Bibliography	15

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[ISO/DIS 17328](https://standards.iteh.ai/catalog/standards/sist/3dfaebae-345a-48c5-8b93-970b7dbeb23e/iso-dis-17328)

<https://standards.iteh.ai/catalog/standards/sist/3dfaebae-345a-48c5-8b93-970b7dbeb23e/iso-dis-17328>

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 172, *Optics and photonics*, Subcommittee SC 03, *Optical materials and components*.

This second edition cancels and replaces the first edition (ISO 17328:2014), which has been technically revised.

The main changes compared to the previous edition are as follows:

- Clarified the description of the device.
- Addition of contents to the test report.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

This International Standard applies to the measurement of relative refractive index to the air for infrared optical materials.

Two major methods for measuring the refractive index of infrared materials exist. These are interferometric methods and minimum deviation methods. In this International Standard, a test method using minimum deviation for infrared materials is described, which is also used in the visible spectral range. It has the advantages of being applicable to more kinds of materials compared with interferometric methods and of ease of data processing because of the simple measurement principle.

iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO/DIS 17328](https://standards.iteh.ai/catalog/standards/sist/3dfaebae-345a-48c5-8b93-970b7dbeb23e/iso-dis-17328)

<https://standards.iteh.ai/catalog/standards/sist/3dfaebae-345a-48c5-8b93-970b7dbeb23e/iso-dis-17328>

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO/DIS 17328

<https://standards.iteh.ai/catalog/standards/sist/3dfaebae-345a-48c5-8b93-970b7dbeb23e/iso-dis-17328>

Optics and photonics — Optical materials and components — Test method for refractive index of infrared optical materials

1 Scope

This International Standard provides a standard method for measuring the relative refractive index to the air of infrared materials used in the infrared spectral range from 0,78 μm to 25 μm .

The scope of this International Standard excludes methods for measuring the refractive index of birefringent materials and methods for measuring the complex refractive index.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 11382:2010, *Optics and photonics — Optical materials and components — Characterization of optical materials used in the infrared spectral range from 0,78 μm to 25 μm*

3 Terms and definitions

For the purposes of this document, the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

3.1

refractive index

absolute refractive index

ratio of the velocity of the electromagnetic waves at a specific wavelength in a vacuum to the velocity of the waves in the medium

[SOURCE: ISO 12123:2018, Terms and [definitions 3.1](#)]

3.2

relative refractive index

ratio of the (absolute) refractive index of the material of the specimen to the (absolute) refractive index of the material in contact with the specimen at a specific wavelength

3.3

angle of minimum deviation

the angle between the ray incident upon the specimen prism and the ray exiting the specimen prism at its minimum value, which occurs when the ray inside the specimen prism makes equal angles with the entrance and the exit faces of the specimen prism

4 Method for measuring

4.1 General

In this International Standard, the technique of the minimum deviation method for measuring refractive index is described.

The minimum deviation method shall be applied for measuring refractive index.

4.2 Principle

As shown in [Figure 1](#), when the monochromatic light beam is refracted by the specimen prism with minimum deviation, the relative refractive index of the specimen prism to the air at the wavelength of the monochromatic light beam is described by the following [formula \(1\)](#):


$$n_{\text{rel}} = \frac{\sin[(\alpha + \delta)/2]}{\sin(\alpha/2)} \quad (1)$$

where

n_{rel} is the relative refractive index of the specimen prism to the air;

α is the apex angle of the specimen prism;

δ is the angle of minimum deviation of the monochromatic light beam refracted by the specimen prism.

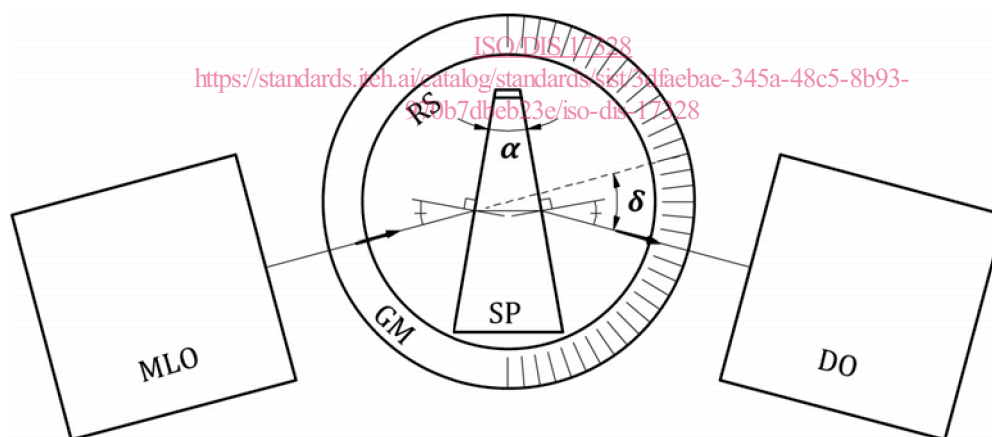

Key

MLO monochromatic light source optics

SP specimen prism

RS rotating stage

GM goniometer


DO detector optics

δ angle of minimum deviation

α apex angle of the specimen prism

Figure 1 — Schematic of the minimum deviation method

The monochromatic light beam shall be parallel to the plane of section, PS, of the specimen prism. (See [4.2, Figure 2](#).)

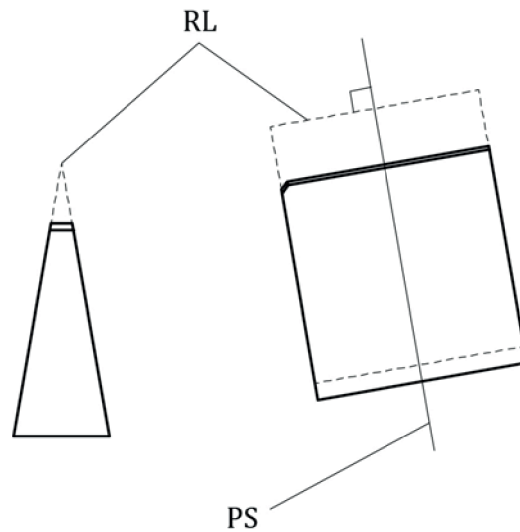**Key**

RL ridge line

PS plane of section

Figure 2 — Ridge line and the plane of section of the specimen prism
 (standards.iteh.ai)

4.3 Apparatus and procedure for measurement

The apparatus for measurement shall be equipped with the following:

- a) a method to emit a collimated monochromatic light beam of specified wavelength to the specimen prism;
- b) a method to vary the angle of the collimated monochromatic light beam to the entrance face of the specimen prism;
- c) a method to determine the direction of the monochromatic light beam refracted by the specimen prism;
- d) a method to indicate the angle of minimum deviation δ ;
- e) a method to measure the temperature of the specimen prism.

Examples of apparatus for measurement of the angle of minimum deviation are shown in [Annex A](#). A procedure for measurement is also described in [Annex A](#). In addition, the absolute value of the angle of deviation error is described in [Annex B](#).

See [4.2, Figure 1](#).

4.4 Wavelength of light beam for measurement

The wavelengths of measurement shall adequately sample the spectral range of interest to enable curve fitting of the data to a dispersion formula, allowing calculation of the relative refractive index at any arbitrary wavelength within the spectral range.

5 Specimens


5.1 The shape and dimensions of the specimen prism

The specimen shall be a wedged prism made of the material to be measured. The entrance face and the exit face shall be polished.

An example of the shape of the specimen prism is shown in Figure 3. The optimum apex angle (such that error in measurement of the apex angle is least severe) for a material of the relative refractive index n_{rel} is

$$\alpha = 2\arctan(1/n_{rel}) \tag{2}$$

For low index materials, this relation may result in undesirably large apex angles; this relation shall be used as guidance.

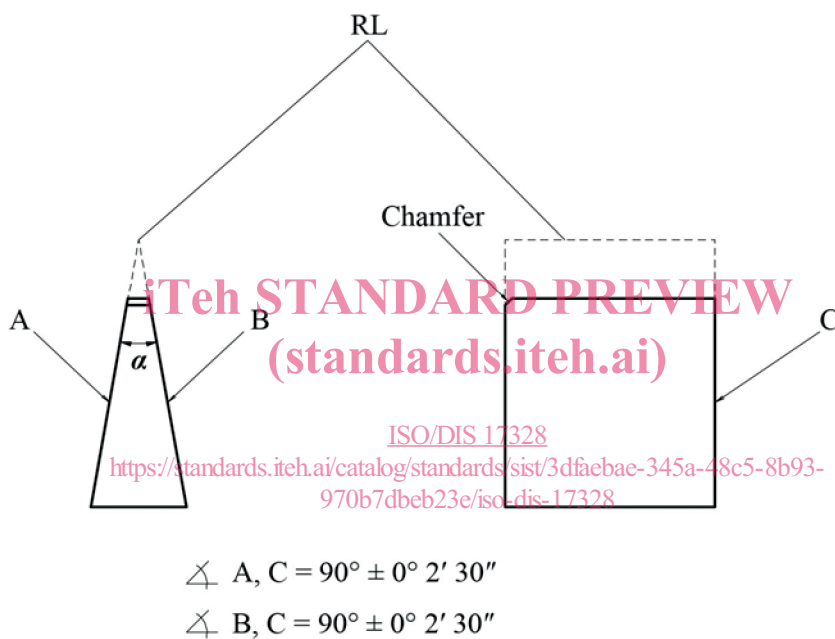

Key

RL ridge line

α apex angle of the specimen prism

Figure 3 — Shape of the specimen prism

5.2 Surface accuracy

The surface accuracy of the entrance face and the exit face of the specimen prism shall be measured with an interferometer. Any measured power term shall not be subtracted from measurement data. A surface flatness error should be 150 nm P-V or less over the entire clear aperture of the specimen prism faces.

6 Test report

The test report shall specify the following:

- a) specimen name in accordance with ISO 11382:2010, 5.6;
- b) date, place, measurer name;

- c) temperature, humidity, air pressure of ambient air;
- d) apex angle of the specimen prism;
- e) temperature of the specimen prism;
- f) surface accuracy of the entrance face and the exit face;
- g) wavelengths and bandwidth (full width at half maximum) of wavelengths for measurement;
- h) angles of minimum deviation;
- i) relative refractive indices to the air.

Values of c), d), e), g), h) and i) shall be specified with values of uncertainty. In the case of the ambient medium is not air, add the name of ambient medium to the report.

Analysis errors are described in [Annex B](#).

iTeh STANDARD PREVIEW (standards.iteh.ai)

[ISO/DIS 17328](#)

<https://standards.iteh.ai/catalog/standards/sist/3dfacebae-345a-48c5-8b93-970b7dbeb23e/iso-dis-17328>