

© ISO 2023/2024

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: + 41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Formatted: Font: 11 pt, Bold

Formatted: Font: 11 pt, Bold

Formatted: HeaderCentered, Space After: 0 pt, Line spacing: single

Formatted: Left: 1.9 cm, Right: 1.9 cm, Bottom: 1 cm, Gutter: 0 cm, Header distance from edge: 1.27 cm, Footer distance from edge: 0.5 cm

Commented [eXtyles1]: The reference is to a withdrawn standard which has been replaced

ISO 20344, Personal protective equipment — Test methods for footwear

Formatted: Default Paragraph Font

Formatted: Indent: Left: 0 cm, Right: 0 cm, Space Before: 0 pt, No page break before, Adjust space between Latin and Asian text, Adjust space between Asian text and numbers

Formatted: French (France)

Formatted: French (France)

Formatted: French (France)

iTeh Standards
(<https://standards.itih.ai>)
Document Preview

ISO/FDIS 6760-1

<https://standards.itih.ai/catalog/standards/iso/af90dc53-5da2-46ab-8a76-ce2df00fb24a/iso-fdis-6760-1>

Formatted: FooterPageRomanNumber

Contents

Forewordv

Introduction.....vi

1 Scope1

2 Normative references1

3 Terms and definitions.....1

4 Principle.....2

5 Measuring apparatus3

5.1 Goniometer3

5.2 Light source3

5.3 Detector.....3

5.4 Thermal chamber.....3

6 Specimen prism.....5

7 Measurement5

7.1 Measurement of apex angle.....5

7.2 Measurement of the angle of minimum deviation.....5

8 Calculation5

8.1 Absolute refractive index5

8.2 Temperature coefficient of absolute refractive index.....7

8.3 Temperature coefficient of relative refractive index.....7

9 How to express the temperature coefficient of refractive index.....9

10 Test report9

Annex A (informative) Formula for calculating the refractive index of air.....10

Annex B (informative) Calculation method for obtaining the relative refractive index of glass at an arbitrary temperature, air pressure and relative humidity13

Annex C (informative) Half prism method16

Annex D (informative) Interpolation formula for $\Delta n/\Delta T$ 21

Annex E (informative) Derivation and verification of $\Delta n_{rel}/\Delta T$ 23

Bibliography.....27

5.1 Goniometer3

5.2 Light source3

5.3 Detector3

5.4 Thermal chamber3

7.1 Measurement of apex angle4

7.2 Measurement of the angle of minimum deviation4

Formatted: Font: 11 pt, Bold

Formatted: Font: 11 pt, Bold

Formatted: HeaderCentered, Left, Space After: 0 pt, Line spacing: single

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers

Formatted: FooterPageRomanNumber

ISO/FDIS 6760-1:20232024(E)

- ~~8.1 Absolute refractive index 4~~
- ~~8.2 Temperature coefficient of absolute refractive index 5~~
- ~~8.3 Temperature coefficient of relative refractive index 6~~

Formatted: Font: 11 pt, Bold

Formatted: Font: 11 pt, Bold

Formatted: HeaderCentered, Space After: 0 pt, Line spacing: single

iTeh Standards
(<https://standards.itih.ai>)
Document Preview

ISO/FDIS 6760-1

<https://standards.itih.ai/catalog/standards/iso/af90dc53-5da2-46ab-8a76-ce2df00fb24a/iso-fdis-6760-1>

Formatted: FooterPageRomanNumber

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO document should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 172, *Optics and photonics*, Subcommittee SC 3, *Optical materials and components*.

A list of all parts in the ISO 6760 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Formatted: Font: 11 pt, Bold

Formatted: Font: 11 pt, Bold

Formatted: HeaderCentered, Left, Space After: 0 pt, Line spacing: single

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers

Formatted: English (United Kingdom)

Commented [eXtyle2]: Invalid reference: "ISO 6760 series"

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: FooterPageRomanNumber

Introduction

Optical glass is widely used in optical devices such as cameras, telescopes, and microscopes, and its refractive index is measured by the minimum deviation method (see ISO 21395-1) and the V-block refractometer method (see ISO 21395-2^[6],^[4]). Here, when designing an optical apparatus that requires high resolution, it is necessary to consider the temperature change of the refractive index of the optical glass in the usage environment, however up until now, there is no ~~international standard~~International Standard. In view of the above situation, this document proposes a method for measuring the temperature coefficient of refractive index of optical glass with high accuracy, aiming to help mutual understanding of measured value users and contribute to efficiency and fairness.

Formatted: Font: 11 pt, Bold

Formatted: Font: 11 pt, Bold

Formatted: HeaderCentered, Space After: 0 pt, Line spacing: single

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

iTeh Standards (<https://standards.itih.ai>) Document Preview

ISO/FDIS 6760-1

<https://standards.itih.ai/catalog/standards/iso/af90dc53-5da2-46ab-8a76-ce2df00fb24a/iso-fdis-6760-1>

Formatted: FooterPageRomanNumber

Optics and photonics — Test method for temperature coefficient of refractive index of optical glasses

Part 1 Minimum deviation method

1 Scope

This document specifies the measurement method used for calculating the temperature coefficient of the refractive index by measuring the refractive index, which changes with the temperature of the optical glass using the minimum deviation method.

The intended temperature range for the specified measurement method is -40 °C to +80 °C.

The intended wavelength range for the specified measurement method is 365 nm to 1 014 nm.

The intended accuracy for the specified measurement method is $1 \times 10^{-6} \text{ K}^{-1}$.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

~~ISO 21395-1:2020, Optics and photonics — Test method for refractive index of optical glasses. Part 1: Minimum deviation method~~

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org>

3.1 temperature coefficient of refractive index

ratio of refractive index change to temperature change at a selected wavelength

Note 1—to entry: Similar to ISO 9802

3.2 temperature coefficient of absolute refractive index

$\Delta n_{\text{abs}} / \Delta T$
ratio of refractive index change in vacuum to temperature change at a selected wavelength

[SOURCE: ISO 9802:2022, 3.4.2.3]

Formatted: Left: 1.9 cm, Right: 1.9 cm, Bottom: 1 cm, Gutter: 0 cm, Section start: New page, Header distance from edge: 1.27 cm, Footer distance from edge: 0.5 cm

Formatted: Main Title 2, Space After: 0 pt, Line spacing: single, Adjust space between Latin and Asian text, Adjust space between Asian text and numbers

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm

Formatted: Default Paragraph Font

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers

Commented [eXtyle3]: The URL <https://www.iso.org/obp> has been redirected to <https://www.iso.org/obp/ui>. Please verify the URL.

Formatted

Formatted

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted

Formatted

Formatted: Regular, Font: Bold

Formatted: Regular Italic, Font: Bold, Not Italic

Formatted

Formatted: Regular, Font: Bold

Formatted: Regular Italic, Font: Bold, Not Italic

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

3.3 temperature coefficient of relative refractive index

ratio of refractive index change at an air pressure of 1,013 3 × 10⁵ Pa and a relative humidity of 0 % to temperature change at a selected wavelength

[SOURCE: ISO 9802:2022, 3.4.2.4, modified: — 1,013 3 × 10⁵ Pa and a relative humidity of 0 %.]

Note 1 to entry: This definition of Δn_{rel}/ΔT is for a specific pressure and humidity. Δn_{rel}/ΔT can be calculated for any other pressure and humidity by understanding the index of air in those conditions.

3.4 thermal chamber

chamber where the temperature of the specimen can be changed and maintained to a preset temperature


4 Principle

As shown in Figure 1, a specimen prism is placed in a thermal chamber. The temperature of the specimen prism is changed from T₁ to T₂ or from T₂ to T₁, and the refractive index of the specimen prism is measured at the temperatures of T₁ and T₂ respectively, in accordance with the method described in ISO 21395-1 to find the temperature coefficient of refractive index. Figure 2 shows the concept of calculating this temperature coefficient of refractive index.

NOTE 1 In this document the term "light" is used to describe not only optical radiation visible to the human eye but also radiation in the infrared and ultraviolet spectrum.

NOTE 2 In this document, all temperature symbols are represented by "T". The original symbol for temperature in ISO 8000-5 is "t" or "θ" for temperature in Celsius degrees, and "T" for absolute temperature.

NOTE 3 Alternatively the measurement principle according to Annex C can be applied.

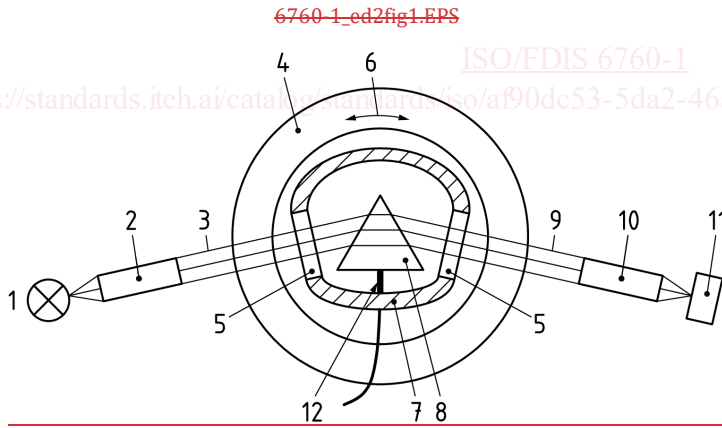

Key	
1	light source
2	collimator
3	incident light
4	lens
5	filter
6	thermal chamber containing the specimen prism
7	specimen prism
8	transmitted light
9	detector
10	scale
11	light source

- Formatted: Font: 11 pt, Bold
- Formatted: Font: 11 pt, Bold
- Formatted: HeaderCentered, Space After: 0 pt, Line spacing: single
- Formatted: Regular, Font: Bold
- Formatted: Regular Italic, Font: Bold, Not Italic
- Formatted: Regular Sub, Font: Bold, Not Superscript/ Subscript
- Formatted: Regular, Font: Bold
- Formatted: Regular Italic, Font: Bold, Not Italic
- Formatted: Default Paragraph Font
- Formatted: Default Paragraph Font
- Formatted: Default Paragraph Font
- Formatted: Default Paragraph Font
- Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm
- Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers
- Formatted: Default Paragraph Font
- Formatted: Default Paragraph Font
- Formatted: Default Paragraph Font
- Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm
- Commented [eXtyle4]: Not found: "ISO 8000-5"
- Formatted: Default Paragraph Font
- Formatted: Default Paragraph Font
- Formatted: Default Paragraph Font


- Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm
- Formatted Table
- Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm
- Formatted
- Formatted: FooterPageRomanNumber

ISO/FDIS 6760-1:2023/2024(E)

- a) ~~a)~~ have the ability to change the temperature of the specimen prism between the temperatures to be measured,
- b) ~~b)~~ have a structure that can maintain the temperature distribution in the specimen within the range of 1,0 K during raising and lowering of the temperature,
- c) ~~c)~~ have a thermometer to measure the temperature of the specimen prism with an accuracy of $\pm 0,2$ K or better,
- d) ~~d)~~ have the ability to provide a vacuum with a residual pressure of less than 10 Pa for the purpose of having a negligible influence of the refractive index of air and of preventing condensation, and
- e) ~~e)~~ have windows made of a parallel plate of quartz glass polished on both sides. The wedge angle between the parallel polished faces shall not exceed 5 arc sec, the flatness of the parallel polished faces shall be $\lambda/10$ or better.

NOTE Quartz glass is used because it has a high transmittance over a wide wavelength range, a high durability against temperature changes, and is resistant to breakage.

6760-1_ed2fig3.EPS

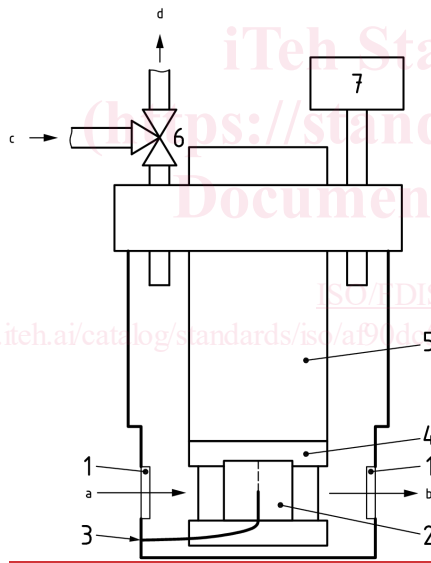

- | | | | |
|---|---|-----|----------------|
| 1 | incident light | 67 | vacuum gauge |
| 2 | outgoing light | 7a | Incident light |
| 3 | thermometer | 9b | Outgoing light |
| 4 | thermal conductor specimen prism holder | 9c | to vacuum pump |
| 5 | heating and cooling unit | 10d | leak inlet |
| 6 | three-way valve | 11 | vacuum gauge |

Formatted: Font: 11 pt, Bold

Formatted: Font: 11 pt, Bold

Formatted: HeaderCentered, Space After: 0 pt, Line spacing: single

Formatted: Numbered + Level: 1 + Numbering Style: a, b, c, ... + Start at: 1 + Alignment: Left + Aligned at: 0 cm + Indent at: 0 cm, Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm

Formatted Table

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 0.7 cm + 1.4 cm + 2.1 cm + 2.8 cm + 3.5 cm + 4.2 cm + 4.9 cm + 5.6 cm + 6.3 cm + 7 cm

Formatted: FooterPageRomanNumber

Figure 3 — Example of thermal chamber

6 Specimen prism

The specimen prism shall be in accordance with ISO 21395-1:2020, Clause 6.

7 Measurement

7.1 Measurement of apex angle

The apex angle of the specimen prism shall be measured in accordance with ISO 21395-1:2020, 8.2.

7.2 Measurement of the angle of minimum deviation

The angle of minimum deviation of the specimen prism shall be measured at two or more temperatures in accordance with ISO 21395-1:2020, 8.3.

The bisector of the apex angle α is parallel to the bisector of the angle δ , formed by the opposite two-surface window of the thermal chamber. (See Figure 4) (See Figure 4)

The degree of vacuum around the specimen prism shall be less than 10 Pa. The minimum deviation angle should be measured at a temperature within $\pm 0,5$ °C with respect to the target temperature.

NOTE 1:— Allowable measurement error is an error in the measurement of the refractive index. When the allowable measurement error is smaller than $0,5 \times 10^{-6}$, the allowable angle difference between the bisectors of α and β is within 2° ; when the allowable measurement error is smaller than $0,5 \times 10^{-5}$, the allowable angle difference between the bisectors of α and β is within 6° .

NOTE 2:— The temperature to be measured is arbitrary. Allow sufficient time for the specimen prism to reach a uniform temperature throughout. In most cases, the temperatures measured are -40 °C, -20 °C, 0 °C, 20 °C, 40 °C, 60 °C and 80 °C.

8 Calculation

8.1 Absolute refractive index

The absolute refractive index at each temperature of the specimen prism shall be calculated by Formula (1) (adaptation of ISO 21395-1:2020, Clause 4).

$$n_{\text{abs}}(T) = \frac{\sin\left[\frac{\alpha + \delta_{\text{min,vac}}(T)}{2}\right]}{\sin\left(\frac{\alpha}{2}\right)} \quad (1)$$

$$n_{\text{abs}}(T) = \frac{\sin\left[\frac{\alpha + \delta_{\text{min,vac}}(T)}{2}\right]}{\sin\left(\frac{\alpha}{2}\right)} \quad (1)$$

where

$n_{\text{abs}}(T)$ is the absolute refractive index of specimen prism at temperature T ;

α is the apex angle of the specimen prism;

$\delta_{\text{min,vac}}(T)$ is the minimum deviation angle at temperature T ;

Formatted: Font: 11 pt, Bold

Formatted: Font: 11 pt, Bold

Formatted

Formatted

Formatted

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted: Default Paragraph Font

Formatted

Formatted Table

Formatted: Font: Not Italic

Formatted

Formatted

Formatted: FooterPageRomanNumber