



SLOVENSKI STANDARD

SIST ISO 11171:2023

01-april-2023

Fluidna tehnika - Hidravlika - Umerjanje naprav za avtomatsko štetje delcev v tekočinah

Hydraulic fluid power - Calibration of automatic particle counters for liquids

iTeh STANDARD PREVIEW

Transmissions hydrauliques - Étalonnage des compteurs automatiques de particules en suspension dans les liquides

Ta slovenski standard je istoveten z: **ISO 11171:2022**

ICS:

17.120.01	Merjenje pretoka tekočin na splošno	Measurement of fluid flow in general
23.100.01	Hidravlični sistemi na splošno	Fluid power systems in general

SIST ISO 11171:2023

en,fr,de

INTERNATIONAL
STANDARD

ISO
11171

Fifth edition
2022-03

**Hydraulic fluid power — Calibration of
automatic particle counters for liquids**

*Transmissions hydrauliques — Étalonnage des compteurs
automatiques de particules en suspension dans les liquides*

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST ISO 11171:2023](https://standards.iteh.ai/catalog/standards/sist/a2635489-c03f-4dfe-9ffa-f71d49e6fbf8/sist-iso-11171-2023)

<https://standards.iteh.ai/catalog/standards/sist/a2635489-c03f-4dfe-9ffa-f71d49e6fbf8/sist-iso-11171-2023>



Reference number
ISO 11171:2022(E)

© ISO 2022

iTeh STANDARD PREVIEW (standards.iteh.ai)

SIST ISO 11171:2023

<https://standards.iteh.ai/catalog/standards/sist/a2635489-c03f-4dfe-9ffa-f71d49e6fbf8/sist-iso-11171-2023>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2022

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

Page

Foreword.....	iv
Introduction.....	vi
1 Scope.....	1
2 Normative references.....	1
3 Terms and definitions.....	1
4 Materials and equipment.....	3
5 Sequence of APC calibration procedures.....	5
6 Sizing calibration procedure.....	9
7 Data presentation.....	19
8 Identification statement.....	20
Annex A (normative) Preliminary APC check.....	21
Annex B (normative) Coincidence error procedure.....	25
Annex C (normative) Flow rate limit determination.....	29
Annex D (normative) Resolution determination.....	34
Annex E (normative) Verification of particle-counting accuracy.....	39
Annex F (normative) Preparation and verification of bottles of secondary calibration suspensions.....	42
Annex G (normative) Dilution of calibration suspension samples.....	46
Annex H (informative) Verification of particle size distribution of calibration samples.....	49
Bibliography.....	51

ISO 11171:2022(E)

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 131 *Fluid power systems*, SC 6, *Contamination control*.

This fifth edition cancels and replaces the fourth edition (ISO 11171:2020), which has been technically revised.

The main changes are as follows:

- in term [3.8](#), particle size distribution, Note 1 to entry has been amended;
- in [6.12](#) c), 0,72 has been changed to 0,56;
- in [6.12](#) d) 1,32 has been changed to 1,56;
- in [B.4](#), 3rd line, “mass concentrate” has been changed to “mass concentration”;
- [B.8](#) has been amended to read: “.....”calculate the theoretical number concentration of particles for each mass concentration, X_t .”;
- in [Table B.1](#), the units for “ X_t (particles/L)” have been corrected to “ X_t (particles/mL)”;
- in [D.3](#) c), 0,72 has been changed to 0,56;
- in [D.3](#) d), 1,32 has been changed to 1,56;
- in [D.7](#) a), 0,72 has been changed to 0,56;
- in [D.7](#) e), 1,32 has been changed to 1,56;
- in [G.6](#), the subscript in the denominator of [Formula G.3](#) has been corrected from “ V_0 ” to “ V_S ”;
- in Reference [\[6\]](#) in the Bibliography, the RM 8631 batch identifier has been changed from “a” to “b”;
- in Reference [\[7\]](#) in the Bibliography, the RM 8632 batch identifier has been changed from “b” to “a”.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

iTeh STANDARD PREVIEW (standards.iteh.ai)

SIST ISO 11171:2023

<https://standards.iteh.ai/catalog/standards/sist/a2635489-c03f-4dfe-9ffa-f71d49e6fbf8/sist-iso-11171-2023>

ISO 11171:2022(E)**Introduction**

In hydraulic fluid power systems, power is transmitted and controlled through a liquid under pressure within an enclosed circuit. The fluid is both a lubricant and a power-transmitting medium. Reliable system performance requires control of the contaminants in the fluid. Qualitative and quantitative determination of the particulate contaminants in the fluid medium requires precision in obtaining the sample and in determining the contaminant particle size distribution and concentration. Liquid automatic particle counters (APC) are an accepted means of determining the concentration and size distribution of the contaminant particles. Individual APC accuracy is established through calibration.

This document is a standard calibration procedure for APC that are used for determining particle sizes and counts. The primary particle-sizing calibration is conducted using NIST SRM 2806x suspensions with particle size distribution certified by the United States National Institute of Standards and Technology (NIST) for particle sizes 30 μm (c) and smaller, and using polystyrene latex spheres at larger sizes.

A secondary calibration method uses suspensions of NIST RM 8631x, ISO MTD, or other test dust conforming to ISO 12103-1, which are independently analysed using an APC calibrated by the primary method. Minimum performance specifications are established for the APC coefficient of variation (CV) of sample volume, CV of flow rate, resolution and particle counting accuracy. The operating limits of an APC, including its threshold noise level, coincidence error limit and flow rate limits are determined.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

[SIST ISO 11171:2023](https://standards.iteh.ai/catalog/standards/sist/a2635489-c03f-4dfe-9ffa-f71d49e6fbf8/sist-iso-11171-2023)

<https://standards.iteh.ai/catalog/standards/sist/a2635489-c03f-4dfe-9ffa-f71d49e6fbf8/sist-iso-11171-2023>

Hydraulic fluid power — Calibration of automatic particle counters for liquids

1 Scope

This document specifies procedures for the following:

- a) primary particle-sizing calibration for particle sizes 1 μm (c) and larger, sensor resolution and counting performance of liquid automatic particle counters that are capable of analysing bottle samples;
- b) secondary particle-sizing calibration using suspensions verified with a primary calibrated APC;
- c) establishing acceptable operation and performance limits;
- d) verifying particle sensor performance using a test dust;
- e) determining coincidence and flow rate limits.

This document is applicable for use with hydraulic fluids, aviation and diesel fuels, engine oil and other petroleum-based fluids. This document is not applicable to particle-sizing calibration using NIST SRM 2806b primary calibration suspensions.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3722, *Hydraulic fluid power — Fluid sample containers — Qualifying and controlling cleaning methods*

ISO 4787, *Laboratory glass and plastic ware — Volumetric instruments — Methods for testing of capacity and for use*

ISO 5598, *Fluid power systems and components — Vocabulary*

ISO 12103-1, *Road vehicles — Test contaminants for filter evaluation — Part 1: Arizona test dust*

ISO 16889, *Hydraulic fluid power — Filters — Multi-pass method for evaluating filtration performance of a filter element*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 5598 and the following apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

3.1

automatic particle counter

APC

instrument that automatically:

ISO 11171:2022(E)

- a) senses individual particles suspended in a controlled volume of fluid using optical light extinction or light scattering principles;
- b) measures the size of particles;
- c) sorts or compiles particles into size ranges;
- d) counts particles in each size range;
- e) reports the number of particles in each size range per unit volume; and
- f) facilitates instrument calibration according to this document.

Note 1 to entry: APC used for *particle size* (3.7) determination with hydraulic fluids, aviation and diesel fuels, engine oil and other petroleum-based fluids shall be calibrated in accordance with [Clause 5](#) of this document.

3.2

threshold noise level

minimum voltage setting of an APC (3.1) at which the observed pulse-counting frequency does not exceed 60 counts/min due to electrical noise in the absence of flow in the *sensing volume* (3.3)

Note 1 to entry: The Brownian motion of any detectable particles in the sensing zone during performance of [subclause A.2](#) can result in erratic results.

3.3

sensing volume

portion of the illuminated region of the sensor through which the fluid stream passes and from which the light is collected by the optical system

3.4

resolution

measure of the ability of an APC (3.1) to distinguish between particles of similar, but different, sizes as determined in accordance with [Annex D](#) of this document

3.5

coincidence error limit

highest concentration of NIST RM 8632x that can be counted with an *automatic particle counter* (3.1) with an error of less than 5 % resulting from the presence of more than one particle in the *sensing volume* (3.3) at one time

3.6

working flow rate

flow rate through the sensor used for sample analysis

3.7

particle size

projected area equivalent diameter of particles as determined by NIST using scanning electron microscopy traceable to SI units through a NIST length standard or using a liquid optical single particle APC (3.1) calibrated according to this document

Note 1 to entry: NIST uses scanning electron microscopy to determine the projected area equivalent diameter of particles in NIST standard reference material 2806x, where x is the letter used by NIST to designate the batch number of the certified *primary calibration* (3.9) suspension.

3.8 particle size distribution

cumulative number concentration of particles larger than a specified size, expressed as a function of *particle size* (3.7)

Note 1 to entry: A certified particle size distribution is one provided by a producer of *primary* (3.9) or *secondary calibration* (3.10) suspensions, and certifies that the particle size distribution reported for the suspensions was determined by NIST or determined according to [Annex F](#) of this document. The particle size distribution of SRM 2806x used for *primary calibrations* (3.9) shall consist of the values for Diameter [$\mu\text{m(c)}$] and the corresponding Cumulative Particle Concentration (part/mL) given in the Certificate of Analysis for Standard Reference Material® 2806x^[5].

Note 2 to entry: Verification of particle size distribution of calibration samples is detailed in [Annex H](#) of this document.

3.9 primary calibration

sizing calibration conducted according to the sizing calibration procedure specified in [Clause 6](#) of this document using NIST standard reference material 2806x for *particle sizes* (3.7) 30 $\mu\text{m(c)}$ and smaller, and using polystyrene latex spheres at larger sizes

Note 1 to entry: For details of NIST standard reference material 2806x, see [4.4](#).

3.10 secondary calibration

sizing calibration conducted using secondary calibration suspensions

Note 1 to entry: The sizing calibration procedure is specified in [Clause 6](#) and the preparation of secondary calibration suspensions is set out in [Annex F](#).

3.11 multi-channel analyser

MCA

electronic device capable of sorting incoming electric pulses according to their amplitude

4 Materials and equipment

4.1 Polystyrene latex spheres that:

- a) are in aqueous suspension;
- b) have a nominal diameter of:
 - 1) 10 μm if used for resolution determination in accordance with [Annex D](#);
 - 2) larger than 30 μm for particle size calibration in accordance with [Clause 6](#) for particle sizes of larger than 30 μm ;
- c) have a coefficient of variation that is less than 5 % where the coefficient of variation is the ratio of the standard deviation of the latex particle diameters in the suspension to their mean particle diameter;
- d) have a certificate of analysis that indicates that the latex spheres mean particle diameter and coefficient of variation were determined using techniques with traceability to national standards.

Once opened, suspensions of polystyrene latex spheres shall be used within three months unless the size distribution and cleanliness of the suspension have been verified.

NOTE 1 The size distribution of polystyrene latex spheres can be verified using the method described in [D.14](#).

NOTE 2 Polystyrene latex spheres in aqueous suspension have a limited shelf life. Shelf life is a function of a variety of factors including temperature and microbial contamination of the suspension.

ISO 11171:2022(E)

4.2 Clean diluent, consisting of the test liquid used in ISO 16889 and containing:

- a) an antistatic additive at such a concentration that resultant conductivity of the clean diluent is $(2\ 500 \pm 1\ 000)$ pS/m at room temperature; and
- b) less than 0,5 % of the number concentration of particles equal to or larger than the smallest particle size of interest expected to be observed in the samples.

4.3 Clean aerosol OT diluent, for use in calibration for particle sizes greater than 30 μm (c) and to determine sensor resolution in [Annex D](#) (the clean diluent specified in [4.2](#) is used for all other operations in this document), which:

- a) is prepared from a concentrate made by adding 120 g of aerosol OT to each litre of clean diluent ([4.2](#)), which is:
 - 1) heated to approximately 60 °C and stirred until no undissolved aerosol OT is visible to the eye; and
 - 2) diluted with clean diluent ([4.2](#)) to a final concentration of 12 g of aerosol OT per litre; and
- b) meets the same cleanliness levels as the diluent specified in [4.2](#).

Aerosol OT (dioctyl sulfosuccinate, sodium salt) is a waxy, hygroscopic solid. If it appears damp, or has absorbed water prior to use, dry it first for at least 18 h at approximately 150 °C.

NOTE In [4.3](#) a) 1), it is critical that all of the aerosol OT be dissolved prior to proceeding to [4.3](#) a) 2). Depending upon the local conditions, complete dissolution can require in excess of 6 hours of heating and stirring as described.

WARNING — Follow the precautions for safe handling and usage described in the safety data sheet (available from the supplier of the aerosol OT).

SIST ISO 11171:2023

4.4 NIST standard reference material 2806x (SRM 2806x) primary calibration suspension, where x is the letter used by NIST to designate the batch number of the certified primary calibration suspension available from NIST, for use in primary calibrations. SRM 2806b shall not be used for calibrations according to this document.

4.5 NIST reference material 8631x (RM 8631x) dust, where x is the letter used by NIST to designate the batch number of the reference material, available from NIST, prepared by drying the dust for at least 18 h at a temperature between 110 °C and 150 °C, for use if secondary calibration is to be performed (see [6.1](#)).

4.6 ISO medium test dust (MTD) or other test dust conforming to ISO 12103-1, dried for at least 18 h at a temperature between 110 °C and 150 °C before use, for use if secondary calibration is to be performed (see [6.1](#)).

4.7 NIST reference material 8632x (RM 8632x) dust, where x is the letter used by NIST to designate the batch number of the reference material, prepared by drying the dust for at least 18 h at a temperature between 110 °C and 150 °C, before use, required for determination of coincidence error limit and in [Annexes A, B, C](#) and [E](#).

NOTE The reference materials specified in [4.4](#), [4.5](#), [4.6](#) and [4.7](#) can change as new batches are produced. Such a change does not affect the particle sizing calibration ([Clause 6](#)), but the ability of an APC to meet the counting accuracy requirements of [E.9](#) can be affected if the batch of RM 8632x used to prepare the samples differs from the batch used to create [Table A.1](#).

4.8 Automatic particle counter for liquids, with bottle sampler with at least 8 channels that can be set at various threshold settings.

4.9 Clean sample containers, with closures (appropriate bottle caps, for example), and **volumetric glassware** of at least class B accuracy as defined in ISO 4787, with cleanliness levels lower than 0,5 % of the number of concentration of particles (larger than the smallest particle size of interest) expected to be observed in the samples, confirmed in accordance with ISO 3722.

4.10 Mechanical shaker, such as a paint or laboratory shaker, suitable for dispersing suspensions.

4.11 Ultrasonic bath, with a power density of 3 000 W/m² to 10 000 W/m² of bottom area.

4.12 Linear-linear graph paper or computer software, for generating graphics.

4.13 Log-log graph paper or computer software, for generating graphics.

4.14 Analytical or electronic balance, with the following minimum specifications:

- a) readability: 0,01 mg;
- b) accuracy (agreement with true mass): $\pm 0,05$ mg;
- c) precision (repeatability): 0,05 mg;
- d) front or side doors and a covered top to eliminate the effect of air currents.

4.15 Secondary calibration suspension, prepared according to [Annex F](#) for use in secondary calibrations. Secondary calibration samples shall not be used for primary calibrations.

5 Sequence of APC calibration procedures

5.1 Conduct the procedures of this Clause when a new APC is received or following the repair or re-adjustment of an APC or sensor as shown in [Table 1](#). See [Figure 1](#) for a recommended sequence of steps to be followed when performing a full calibration on a new APC. [Annexes A](#) and [B](#) shall be performed prior to proceeding to [Clause 6](#). Proceed to [Clause 6](#) if neither the APC nor the sensor has been repaired or readjusted, if no detectable change in the operating characteristics has occurred since the last sizing calibration was performed, and if the APC has been subjected to the procedures in [Annexes A, B, C, D](#), and [E](#) and the results have been documented. The specific order of annexes and clauses given in [Figure 1](#) and [Table 1](#) are recommendations. The operator may follow a different order, as long as all required parts are performed.

[Annexes A, B, C, D](#) and [E](#) may be performed by an individual laboratory or by the manufacturer of the APC prior to delivery. If these are performed prior to delivery, it is not always required to repeat these annexes upon receipt of the APC, depending upon the manufacturer's recommendations.

NOTE For the purposes of this subclause, repair or re-adjustment of an APC refers to service or repair procedures that affect the ability of the APC to accurately size and count particles.

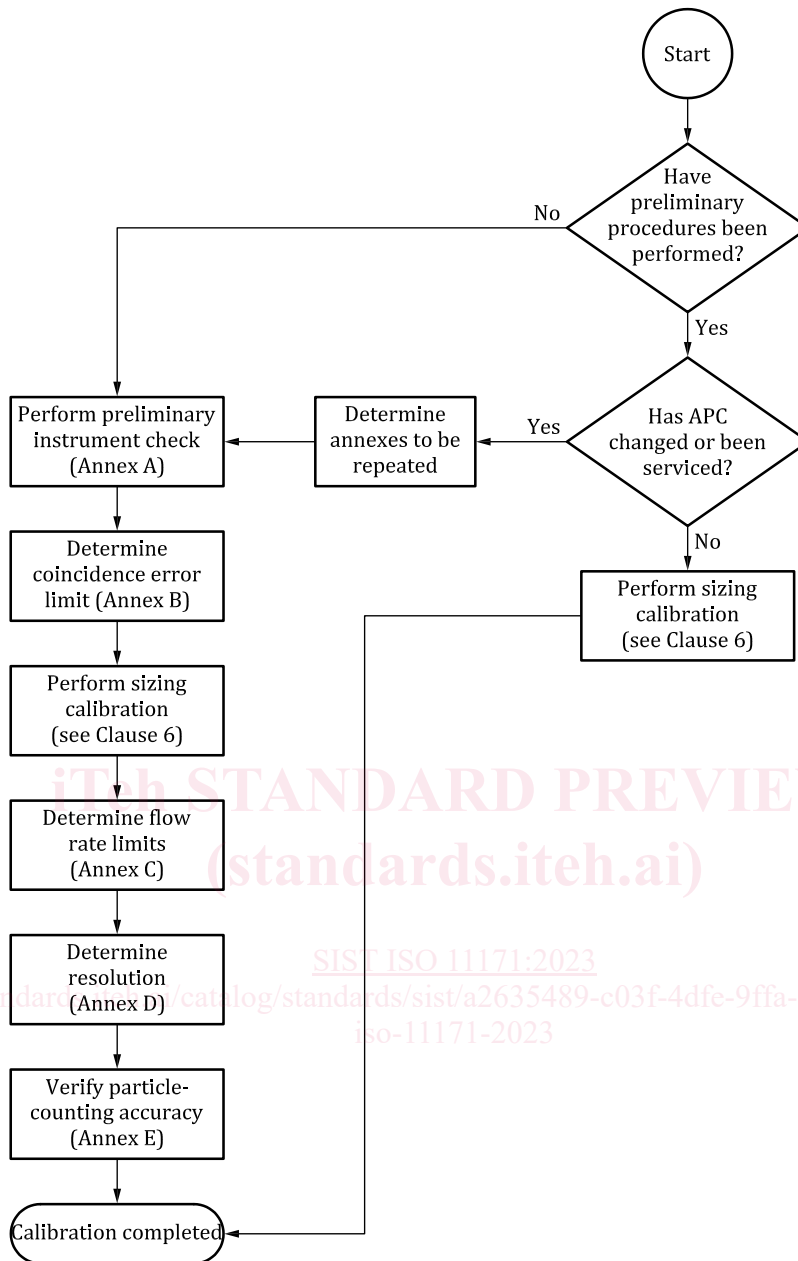


Figure 1 — Recommended sequence of APC calibration procedures

A change in the operating characteristics of the APC can be detected by several different methods, including but not limited to the following:

- using particle data from control samples collected over time and a statistical process control chart, such as an individual moving range (IMR) chart, to detect significant changes in calibration;
- comparing calibration curves reporting particle size in units of $\mu\text{m}(c)$ over time to detect a significant change in calibration;
- returning the APC to its manufacturer for evaluation and assessment of the change in calibration;

- d) analysing a primary or secondary calibration suspension in accordance with [6.5](#) through [6.7](#), then comparing the resulting particle concentration data to the corresponding particle size distribution for the sample:
- 1) if the results agree within the limits for the maximum allowable D_Q ([6.6](#)) given in [Table C.2](#), the ability of the APC to size and count particles has not been significantly affected;
 - 2) if the results do not agree, a significant change has occurred, so proceed as indicated in [Table 1](#).
- e) determining the threshold noise level of the APC in accordance with [A.2](#), then comparing the resulting noise level to previously obtained results. If the threshold noise level has increased by more than 30 % since the last time it was determined, this can be an indication that the calibration of the APC has changed and the APC is in need of repair. If the threshold noise level has not changed, this is not proof that the APC's operating characteristics are unchanged.

If the light source or any part of the optics is adjusted, repaired or replaced, repeat the procedures of [Clause 6](#) and [Annexes A, B, D, and E](#).

If the sensor or counting electronics is adjusted, repaired or replaced, repeat the procedures of [Clause 6](#) and [Annexes A, B, C, D, and E](#).

If the volume measurement system is repaired, replaced or re-adjusted, the procedures of [A.3](#) to [A.9](#) and of [Annex C](#) shall be performed.

It is not necessary to repeat these procedures following normal cleaning procedures, the attachment of cables or peripheral equipment, the replacement of plumbing lines or connections, or following other operations that do not involve disassembly of the APC, sensor or volume measurement system.

5.2 Perform the preliminary APC check, which includes volume accuracy, in accordance with [Annex A](#).

5.3 Determine the coincidence error limits of the APC in accordance with [Annex B](#).

5.4 Perform the sizing calibration procedure in accordance with [Clause 6](#).
<https://standards.iteh.ai/catalog/standards/sist/a2635489-c03f-4dfe-9ffa-f71d49e6fbf8/sist->

5.5 Determine the flow rate limits of the APC in accordance with [Annex C](#).

5.6 Determine the APC resolution in accordance with [Annex D](#).

5.7 Verify the particle-counting accuracy in accordance with [Annex E](#).

5.8 In order to conform to the requirements of this document, the APC shall:

- a) be calibrated in accordance with [5.4](#);
- b) meet the volume accuracy, resolution and sensor performance specifications determined in [5.2](#), [5.6](#) and [5.7](#);
- c) be operated using the calibration curve determined in accordance with [5.4](#) within the coincidence error and flow rate limits determined in accordance with [5.3](#) and [5.5](#).