



Designation: **G138—06 G138 – 12**

Standard Test Method for Calibration of a Spectroradiometer Using a Standard Source of Irradiance¹

This standard is issued under the fixed designation G138; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

INTRODUCTION

A standardized means of performing and reporting calibration of the spectroradiometer for spectral irradiance measurements is desirable.

This test method presents specific technical requirements for a laboratory performing calibration of a spectroradiometer for spectral irradiance measurements. A detailed procedure for performing the calibration and reporting the results is outlined.

This test method for calibration is applicable to spectroradiometric systems consisting of at least a monochromator, input optics, and an optical radiation detector, and applies to spectroradiometric calibrations performed with a standard of spectral irradiance with known irradiance values traceable to a national metrological laboratory that has participated in intercomparisons of standards of spectral irradiance. The standard must also have known uncertainties and measurement geometry associated with its irradiance values.

1. Scope

1.1 This test method covers the calibration of spectroradiometers for the measurement of spectral irradiance using a standard of spectral irradiance that is traceable to a national metrological laboratory that has participated in intercomparisons of standards of spectral irradiance.

1.2 This method is not limited by the input optics of the spectroradiometric system. However, choice of input optics affects the overall uncertainty of the calibration.

1.3 This method is not limited by the type of monochromator or optical detector used in the spectroradiometer system. Parts of the method may not apply to determine which parts apply to the specific spectroradiometer being used. It is important that the choice of monochromator and detector be appropriate for the wavelength range of interest for the calibration. Though the method generally applies to photodiode array detector based systems, the user should note that these types of spectroradiometers often suffer from stray light problems and have limited dynamic range. Diode array spectroradiometers are not recommended for use in the ultraviolet range unless these specific problems are addressed.

1.4 The calibration described in this method employs the use of a standard of spectral irradiance. The standard of spectral irradiance must have known spectral irradiance values at given wavelengths for a specific input current and clearly defined measurement geometry. Uncertainties must also be known for the spectral irradiance values. The values assigned to this standard must be traceable to a national metrological laboratory that has participated in intercomparisons of standards of spectral irradiance. These standards may be obtained from a number of national standards laboratories and commercial laboratories. The spectral irradiance standards consist mainly of tungsten halogen lamps with coiled filaments enclosed in a quartz envelope, though other types of lamps are used. Standards can be obtained with calibration values covering all or part of the wavelength range from 200 to 4500 nm.

¹ This test method is under the jurisdiction of ASTM Committee G03 on Weathering and Durability and is the direct responsibility of Subcommittee G03.09 on Radiometry. Current edition approved June 1, 2006. Published July 2006. Originally approved in 1996. Last previous edition approved in 2003 as G138 – 03. DOI: 10.1520/G0138-06.

1.5 This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.²

2. Referenced Documents

2.1 ASTM Standards:³

E772 Terminology of Solar Energy Conversion

E1341 Practice for Obtaining Spectroradiometric Data from Radiant Sources for Colorimetry

2.2 Other Documents:

CIE Publication No. 63⁴ The Spectroradiometric Measurement of Light Sources

NIST Technical Note 1927: Guidelines for Evaluation and Expressing Uncertainty of NIST Measurement Results⁵

3. Terminology

3.1 General terms pertaining to optical radiation and optical measurement systems are defined in Terminology . Some of the more important terms from that standard used in this paper are listed here.

3.1.1 *bandwidth, n*—the extent of a band of radiation reported as the difference between the two wavelengths at which the amount of radiation is half of its maximum over the given band.

3.1.2 *diffuser, n*—a device used to scatter or disperse light usually through the process of diffuse transmission or reflection.

3.1.3 *integrating sphere, n*—a hollow sphere coated internally with a white diffuse reflecting material and provided with separate openings for incident and exiting radiation.

3.1.4 *irradiance, n*—radiant flux incident per unit area of a surface.

3.1.5 *monochromator, n*—with respect to optical radiation, the restriction of the magnetic or electric field vector to a single plane; an instrument for isolating narrow portions of the optical spectrum of a light source

3.1.6 *polarization, n*—with respect to optical radiation, the restriction of the magnetic or electric field vector to a single plane.

3.1.7 *radiant flux, n*—the time rate of flow of radiant energy measured in watts.

3.1.8 *spectral irradiance, n*—irradiance per unit wavelength interval at a given wavelength.

3.1.9 *spectroradiometer, n*—an instrument for measuring the radiant energy of a light source at each wavelength throughout the spectrum.

3.1.10 *ultraviolet, adj*—optical radiation at wavelengths below 400 nanometres.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *calibration subsystems, n*—the instruments used to supply and monitor current to a standard lamp during calibration, consisting of a DC power supply, a current shunt, and a digital voltmeter.

3.2.2 *National Metrological Institution (NMI), n*—A nation's internationally recognized standardization laboratory.

² Available from Secretary, U.S. National Committee, CIE, National Institute of Standards and Technology, Gaithersburg, MD 20899; the CIE, (International Commission on Illumination), <http://www.techstreet.com/ciegate.tmpl> CIE Central Bureau, Kegelegasse 27, A-1030 Vienna, Austria.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

⁴ G03

⁵ Available from American National Standards Institute, 11 West 42nd Street, 13th Floor, New York, NY 10036

3.2.2.1 Discussion—

The International Bureau of Weights and Measurements (abbreviation BIPM from the French terms) establishes the recognition through Mutual Recognition Agreements. See <http://www.bipm.org/en/cipm-mra>. The NMI for the United States of America is the National Institute for Standards and Technology (NIST).

3.2.3 *passband, n*—the effective bandwidth (c.f.), or spectral interval, over which the spectroradiometer system transmits at a given wavelength setting. Expressed as full-width at one-half maximum, as in bandwidth. A function of the linear dispersion (nm/mm) and slit or aperture widths (mm) of the monochromator system.

3.2.4 *primary standard of spectral irradiance, n*—a broad spectrum light source with known spectral irradiance values at various wavelengths which are traceable to a national metrological laboratory that has participated in intercomparisons of standards of spectral irradiance.

3.2.5 *responsivity, n*—symbol $R = dS/d\phi$, S is signal from spectroradiometer detector, ϕ is radiant flux at the detector.

3.2.6 *secondary standard of spectral irradiance, n*—a standard calibrated by reference to another standard such as a primary or reference standard.

3.2.7 *slit scattering function, n*—symbol $Z(\lambda_0, \lambda)$, the responsivity of the combined detector and monochromator system as a function of wavelengths, λ , in the neighborhood of a given wavelength setting, λ_0 . The slit scattering function is the spectral responsivity in the neighborhood of specific wavelength setting, λ_0 .

3.2.8 *spectral scattering (stray light), n*— light with wavelengths outside the passband of a spectroradiometer a particular wavelength setting that is received by the detector and contributes to the output signal.

4. Significance and Use

4.1 This method is intended for use by laboratories performing calibration of a spectroradiometer for spectral irradiance measurements using a spectral irradiance standard ~~of~~with known spectral irradiance values and associated uncertainties traceable to a national metrological laboratory that has participated in intercomparisons of standards of spectral irradiance, known uncertainties and known measurement geometry.

4.2 This method is generalized to allow for the use of different types of input optics provided that those input optics are suitable for the wavelength range and measurement geometry of the calibration.

4.3 This method is generalized to allow for the use of different types of monochromators provided that they can be configured for a bandwidth, wavelength range, and throughput levels suitable for the calibration being performed.

4.4 This method is generalized to allow for the use of different types of optical radiation detectors provided that the spectral response of the detector over the wavelength range of the calibration is appropriate to the signal levels produced by the monochromator.

5. Apparatus

5.1 Laboratory:

5.1.1 The room in which the calibrations are performed and especially the area surrounding the optical bench should be devoid of reflective surfaces. The calibration values assigned to the spectral irradiance standard are for direct irradiance from the lamp and any radiation entering the monochromator from some other source including ambient reflections will be a source of error.

5.1.2 The temperature and humidity in the laboratory shall be maintained so as to agree with the conditions under which the calibrations of the spectral irradiance standard and the calibration subsystems were performed (typically 20°C, 25°C, 50 % relative humidity).

5.1.3 Air drafts in the laboratory should be minimized since they could affect the output of electrical discharge lamps.

5.2 Spectroradiometer

5.2.1 Monochromator:

5.2.1.1 This can be a fixed or scanning, single or multiple, monochromator employing holographic or ruled gratings or prisms or a combination of these dispersive elements. For improved performance in the ultraviolet (uv)(UV) portion of the spectrum, it is recommended that a scanning double monochromator be used to achieve lower stray light levels (see Fig. 1). If the monochromator has interchangeable slits, it is important that the manufacturer document the effective bandwidth of the monochromator with all possible combinations of the slits or that these bandwidths be determined experimentally. Configuration of the slits should be such that the bandpass function of the monochromator is symmetric, preferably triangular. The bandwidth should be constant across the wavelength region of interest and maintained between 85 % and 100 % of the measurement wavelength interval. The precision of the wavelength positioning of the monochromator should be 0.1 nm with an absolute accuracy of better than 0.5 nm (see Practice E1341). For improved performance in the uv, it is recommended that high order rejection filters be inserted in the optical path in the monochromator. The purpose of the high order rejection filters is to block radiation in the monochromator of unwanted wavelengths that could otherwise overpower the signals being measured. The effects of variations in temperature and humidity on the performance of the monochromator should be addressed in writing by the manufacturer.

5.2.1.2 ~~Avoid mechanical shock and excessive vibration to the monochromator.~~The monochromator shall not be subject to shock or mechanical vibration during the calibration. This can be facilitated by the use of a vibration isolated lab table. If any optical parts in the monochromator are configurable by the user, refer to the manufacturer precautions about opening the monochromator and handling any parts therein.

5.2.2 Optical Radiation Detector:

5.2.2.1 The optical radiation detector employed by the spectroradiometer ~~should~~shall be selected for optimal response over the wavelength range of interest. It is also important that the detector is sensitive enough to measure the levels of light that will be produced by the monochromator when it is configured for the calibration process. The active area of the detector ~~should~~shall be evenly illuminated by the radiation leaving the exit slit of the monochromator. A photomultiplier is typically used because of its high responsivity and good signal-to-noise ratio. For this reason it is recommended for use when measuring spectral irradiance in the uv portion of the spectrum.

5.2.2.2 ~~The~~Any effects of variation in temperature and humidity on the response of the detector ~~should be~~documented by the ~~manufacturer.~~manufacturer shall be reported. Of all components of the spectroradiometer, the detector is usually the most sensitive

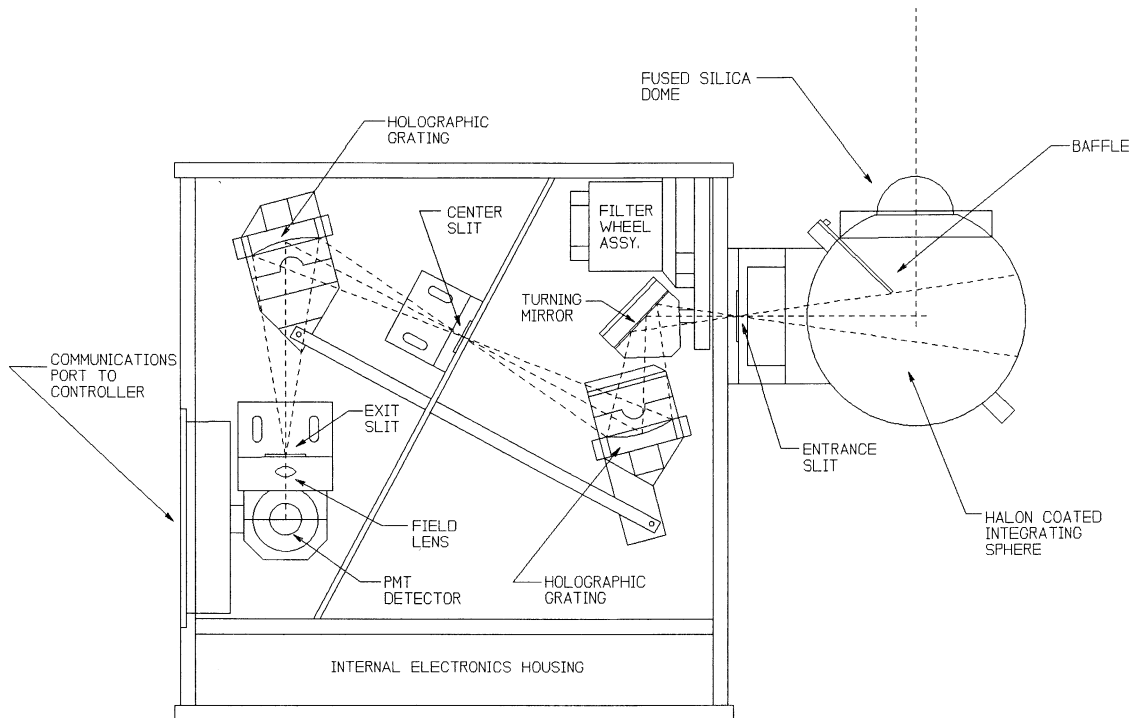


FIG. 1 Typical Double Grating Monochromator Layout (courtesy Optronic Laboratories, Used with Permission)

to changes in temperature. Some detectors may require cooling in order to maintain a specific temperature. Avoid mechanical shock to the detector. If the detector requires an amplifier, any reported limitations and uncertainties in the detector system must factor in the contribution of the amplifier.

5.2.3 If a diode array based spectroradiometer system is used, note the following ~~recommendations-precautions~~:

5.2.3.1 The diode array spectroradiometer should employ internal focusing optics ~~in within~~ the monochromator.

5.2.3.2 When measuring in the ultraviolet, ~~the method of stray light should be controlled~~ control, such as by the use of high order rejection filters or internal baffling, or ~~both-both~~, shall be documented.

5.2.3.3 ~~The~~ It is highly recommended that diode array spectroradiometers spectroradiometers should not be used for measurements below 300 ~~nm-nm~~ without extensive characterization of stray light characteristics and detector performance.

5.2.4 *Input Optics:*

5.2.4.1 Some means of collecting the incident radiation and guiding it to evenly fill the entrance slit of the monochromator is required. The input optics also can serve several other important purposes.

(1) *Cosine Receptor*—~~An ideal~~ Ideally, a cosine receptor will accept all radiation from an entire hemisphere and sample radiant flux according to the cosine of the incident angle.

(2) *Depolarizer*—The components in the monochromator are unfavorably affected by polarized light. A depolarizer such as integrating sphere can produce more consistent results from light sources of any polarization type.

(3) *Diffuser*—A diffuser can remove hotspots from the incident radiation field and produce even illumination on the entrance slit. It can also serve to depolarize optical radiation.

5.2.4.2 Reflective input optics are more desirable than transmissive optics as they perform all three of the functions previously discussed and are generally more useful over larger wavelength ranges. It is important to take into account the amount of attenuation caused by the input optics as this will affect the signal levels at the detector. Ensure that the input optics are suitable for the wavelength range of interest. The predominant choice of input optics is the integrating sphere.

5.3 *Wide-band Cut-on and Cut-off Filters:*

5.3.1 Wideband cut-on and cut-off ~~filters, filters~~ transmit radiation of longer or shorter wavelengths, respectively, than the indicated (cut-on/-off) wavelengths. These are also known as long-pass or short-pass filters. Such filters are needed to establish the level of stray light in the monochromator. The monochromator is set to a given wavelength in a region where the transmission of the filter is negligible (zero), but has high transmittance in nearby band above (for cut-on filter) or below (for cut-off filter) the test wavelength.

5.3.2 Compare the signal from the detector with the filter in place to the shuttered, or dark signal of the detector. A signal between 10 % and 90 % of the unfiltered signal indicates significant scattered light is reaching the detector, possibly due to a non-light-tight enclosure.

5.4 *Optical Radiation Sources*

5.4.1 *Wavelength Calibration Source:*

5.4.1.1 A stable wavelength source is required to calibrate the wavelength positioning accuracy of the monochromator. This can be a gas discharge lamp or a laser. The important thing is that the source have a known spectral emission line(s) of narrow bandwidth.

5.4.1.2 If a laser source is used, occupants of the room should wear eye protection appropriate for the class of laser. Lasers should always be shielded from direct eye view.

5.4.2 *Standard of Spectral Irradiance:*

5.4.2.1 The spectral irradiance standard is a critical component in the calibration process. This standard ~~should~~shall be obtained from a national standards laboratory or a certified commercial laboratory. It must have known spectral irradiance values over the wavelength range of interest. Uncertainties for these spectral irradiance values must also be known in order to compute the total uncertainty of the calibration outlined in this method. The conditions (temperature, relative humidity, calibration distance from the reference plane, orientation and polarity of the lamp current input leads or contacts) under which the standard was calibrated by the supplier must be clearly stated and duplicative. Specifically, the current to the lamp and the measurement geometry must be reported by the supplier in a written document or calibration certificate. The calibration certificate should also contain a physical description of the lamp including materials used in its construction and electrical rating. A unique serial number identifying the standard should also be in the certificate, along with a record of the date on which it was calibrated, and a reference to a specific national metrological laboratory that has participated in intercomparisons of standards of spectral irradiance standard for traceability. Fig. 2 shows the spectral irradiance distribution of a typical tungsten halogen irradiance standard, often used for irradiance calibration over the wavelength range indicated.

5.4.2.2 Care should be exercised when handling the spectral irradiance standard. It should never be necessary to touch the envelope of the lamp. If the envelope is accidentally touched, carefully clean the lamp with denatured alcohol or other appropriate optical cleaner. Never move the lamp when it is lighted. Avoid mechanical shock to the lamp. The lamp ~~should be turned on and off slowly (15 to 30 s); current should be ramped up slowly over a period of 10 to 15 seconds to avoid thermal shock to the filament and possible filament breakage.~~ Monitor the lamp current and only perform calibration measurements while the current is stable within a tolerance of +/-0.05% (or less) of the recommended operating current. When not in use, store the lamp in a dust-free enclosure-enclosure in the geometry (for example, bulb vertical) recommended by the provider of the lamp.

5.4.2.3 The spectral irradiance standard requires recalibration or replacement after ~~50 h of use; a stated period of use stated by the lamp supplier (for example, "50 Hr", as stated for NIST spectral irradiance standard lamps).~~ For this reason, it is important to keep a record of the amount of time the standard is used during each calibration. The time to ramp the lamp current up and down and reach the stability criteria of 5.4.2.2 are not counted as part of this "period of use". [1]

5.4.3 *Secondary Standards of Spectral Irradiance (Control Standards):*

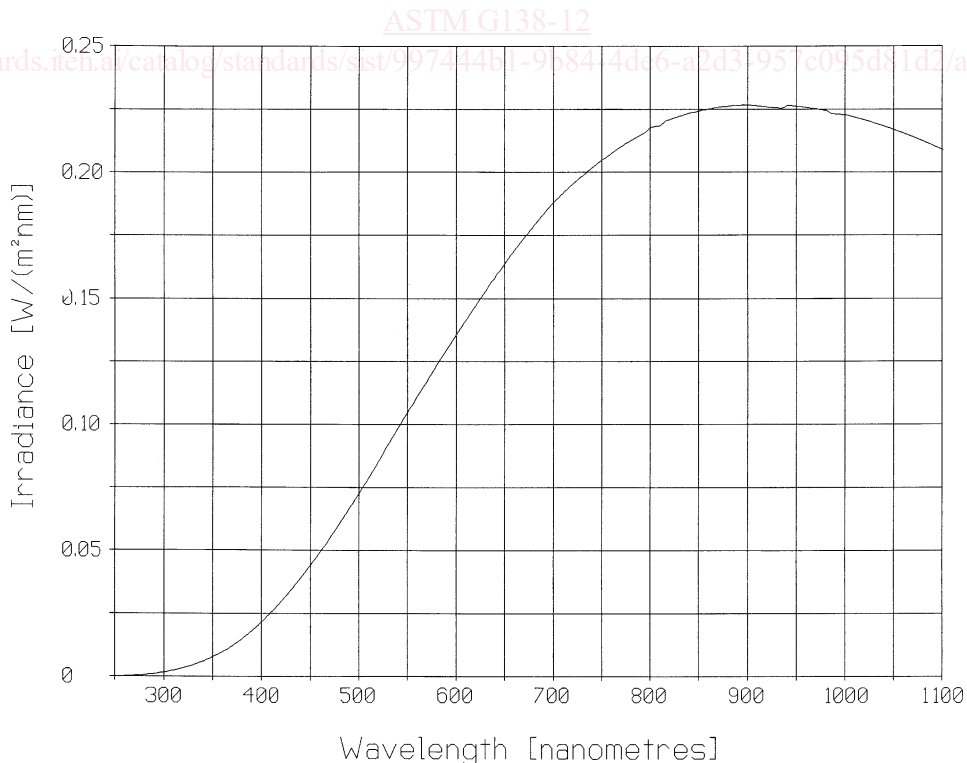


FIG. 2 Spectral Irradiance of Typical Tungsten Filament Quartz Halogen Irradiance Standard

5.4.3.1 The laboratory shall maintain control standards that are of the same type and optical spectral distribution as the primary standard. At least three control standards shall be kept at all times with traceability ~~to a national metrological laboratory through a primary standard of spectral irradiance from an NMI that has participated in intercomparisons of standards of spectral irradiance through the primary standard.~~ irradiance. The control standards shall be measured as soon as possible after the primary standard is assigned calibration values. In addition, regularly scheduled measurements of the control standards will be used to determine the long-term reproducibility of the calibration system, which will be used in determining the calibration uncertainty. If any of the standards, secondary or primary, should vary from its initial calibrated values at any point throughout the spectrum by more than 5 %, the lamp should be replaced.

5.4.4 Use of Secondary Standards as Calibration Reference

5.4.4.1 Secondary standards are to be calibrated through the primary standard. In many cases, manufacturers of spectral irradiance standards can supply the same type of lamp used for the standard without calibration values at a significantly reduced price.

5.4.4.2 Secondary standard lamps must go through a burn-in process, as the manufacturer most likely will not have performed this. Run the lamp at its rated current level for 24 h. After this period, continue running the lamp for an additional 8- h period while regularly monitoring its irradiance in 1-h intervals. If at any point during that 8 h, drift of more than 1 % occurs at any wavelength, discard the lamp and use a different one for a secondary standard.[1]

5.4.4.3 In some cases, it may be desirable and cost-efficient to use the primary standard to regularly calibrate secondary standards and then use the secondary standards for daily calibrations of the spectroradiometer.

5.4.4.4 Previous sections of this standard are explicitly written for calibrations based on a primary standard. When using a secondary standard as a standard for the calibration, the following changes or additions must be made to the calibration method thus far described:

Apparatus-The care and handling of secondary standards should be identical to that of a primary standard.

Report-Additional information for the transfer calibration will be necessary. Everything that was listed for the primary standard can be reclassified as information that should be available if requested. The information that was previously required for the primary standard should now be required for the secondary standard.[1,4,5]

Precision and Bias-The uncertainty calculations should reflect the additional step in the calibration transferring from primary to secondary standard.

5.5 Power Supply System for Spectral Irradiance Standard

5.5.1 Stable DC Power Supply:

5.5.1.1 This is required to power the spectral irradiance standard during the calibration process.

5.5.2 Current Shunt:

5.5.2.1 This is required to accurately monitor the current to the spectral irradiance standard. The current shunt must be calibrated by a laboratory capable of performing calibrations that are traceable to a national metrological laboratory that has participated in intercomparisons of standards of spectral irradiance. ~~an NMI.~~ Documentation must be provided for the calibration of the current shunt including a record of the calibration date, the next due calibration ~~date and the uncertainty~~ date, uncertainty, and traceability of the calibration.

5.5.3 Voltmeter:

5.5.3.1 A precise digital voltmeter (at least 4½ digit) is used in conjunction with the current shunt to accurately monitor the current to the irradiance standard during the calibration process. The current must be monitored extremely closely as a 0.1 % error in the current to the lamp can result in a variation in irradiance of greater than 1 % in the uv portion of the spectrum. The voltmeter must be calibrated by a laboratory capable of performing calibrations that are traceable to a national metrological institute who has participated in intercomparisons of this type. ~~an NMI.~~ The calibration documentation must list the calibration date, the next due calibration date, uncertainty, and ~~the uncertainty~~ traceability of the calibration.

5.6 Optical Bench:

5.6.1 A sturdy surface on which to mount the input optics, monochromator, and spectral irradiance standard is required. Any necessary mounting hardware should be adjustable and lockable.

5.7 Lamp Fixture:

5.7.1 A fixture for holding the spectral irradiance standard is required. The fixture should be designed for the specific lamp type of the spectral irradiance standard. The fixture should hold the lamp securely in place so as to orient the lamp in the same manner each time it is mounted.

5.8 Narrow Band Monochromatic Source:

5.8.1 A source of essentially monochromatic light is needed to determine the slit scattering function of the Spectroradiometer. Spectral bandwidth of the “monochromatic” source should be no more than 20 % of the nominal bandwidth of the Spectroradiometer. Preferable is an amplitude-stabilized wavelength-tuneable laser. Acceptable alternatives are wavelength calibration emission lamps. These lamps contain certain materials that when excited produce well defined and documented spectral emission lines at specific wavelengths depending on the material. Examples include mercury (vapor), xenon, krypton, etc. Note the wavelength calibration source described in 5.3.1 may be used as long as the amplitude of emission lines is stable to within 5 %.