



FINAL DRAFT International Standard

ISO/FDIS 33403

Reference materials — Requirements and recommendations for use

*Matériaux de référence — Exigences et recommandations pour
l'utilisation*

ISO/TC 334

Secretariat: **SABS**

Voting begins on:
2024-02-02

Voting terminates on:
2024-03-29

iTech Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO/FDIS 33403](#)

<https://standards.iteh.ai/catalog/standards/iso/71b53ba4-41d1-49b0-95f8-bd7ee0a5a144/iso-fdis-33403>

RECIPIENTS OF THIS DRAFT ARE INVITED TO SUBMIT, WITH THEIR COMMENTS, NOTIFICATION OF ANY RELEVANT PATENT RIGHTS OF WHICH THEY ARE AWARE AND TO PROVIDE SUPPORTING DOCUMENTATION.

IN ADDITION TO THEIR EVALUATION AS BEING ACCEPTABLE FOR INDUSTRIAL, TECHNOLOGICAL, COMMERCIAL AND USER PURPOSES, DRAFT INTERNATIONAL STANDARDS MAY ON OCCASION HAVE TO BE CONSIDERED IN THE LIGHT OF THEIR POTENTIAL TO BECOME STANDARDS TO WHICH REFERENCE MAY BE MADE IN NATIONAL REGULATIONS.

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

ISO/FDIS 33403

<https://standards.iteh.ai/catalog/standards/iso/71b53ba4-41d1-49b0-95f8-bd7ee0a5a144/iso-fdis-33403>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2024

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Symbols	2
5 Conventions	2
6 RMs and their role in measurement	3
6.1 Common applications of RMs.....	3
6.2 Property values.....	5
6.2.1 General.....	5
6.2.2 Specification of the property.....	5
6.3 Uncertainty statement.....	6
6.4 Traceability statement.....	7
7 Handling of RMs and CRMs	8
8 Assessment of precision	8
8.1 General.....	8
8.2 Number of replicate measurements.....	9
8.3 Requirements with respect to the RM.....	9
8.4 Measurement.....	10
8.5 Data treatment.....	10
8.6 Calculation and assessment of precision.....	11
9 Bias assessment	11
9.1 General.....	11
9.2 Approach to bias checking.....	12
9.3 Utilizing bias data.....	12
10 Calibration	13
10.1 General.....	13
10.2 Practical considerations for calibration.....	14
10.3 Calibration models.....	14
11 Assigning values to other materials	14
11.1 General.....	14
11.2 Pure substances.....	15
11.3 Preparation of calibrants.....	16
12 Conventional scales	17
13 Selection of RMs and CRMs	18
13.1 General.....	18
13.2 Selection of a CRM.....	19
13.3 Selection of RMs.....	20
13.4 Relevance to the measurement system.....	21
Annex A (informative) Calibration models and associated uncertainty models	22
Annex B (informative) Decision errors	25
Annex C (informative) Example of conventional scales	26
Bibliography	27

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 334, *Reference materials*.

This first edition cancels and replaces ISO Guide 33:2015, which has been technically revised.

The main changes are as follows:

- title modified; [ISO/FDIS 33403](https://standards.iteh.ai/catalog/standards/iso/71b53ba4-41d1-49b0-95f8-bd7ee0a5a144/iso-fdis-33403)
- 1.5 removed; <https://standards.iteh.ai/catalog/standards/iso/71b53ba4-41d1-49b0-95f8-bd7ee0a5a144/iso-fdis-33403>
- 5.3 and 5.4 removed;
- [Figure 1](#) revised and explanation inserted;
- [6.1.4](#): former [Annex A](#) Table A.1 inserted as [Table 1](#);
- [9.1.3](#) removed;
- [9.2.1](#) revised;
- [9.3.1](#) and [9.3.2](#) revised and merged into [9.3.1](#)
- [10.2.1](#) moved to [10.1.1](#) and former [10.1.1](#) added as [10.1.2](#);
- [12.2](#) and [12.3](#) moved into the new [Annex C](#);
- former [Annex B](#) now [Annex A](#);
- former [Annex C](#) now [Annex B](#);
- Bibliography revised.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

This document provides general recommendations on the use of reference materials (RMs). These recommendations are exemplified by real-world examples, which to some degree also reflect the level of complexity associated with RMs. This level of detail is deemed to be useful for users of RMs and anyone who has a responsibility in the quality management in laboratories, e.g. drafters, reviewers, managers and assessors of procedures, working instructions and standard operating procedures.

For certified reference materials (CRMs), the metrological traceability of the property values to international scales or other measurement standards has been established. For RMs that are not CRMs, this kind of traceability of property values has often not been established. Nevertheless, these RMs can still be used for assessing parts of measurement procedures, including evaluating various levels of precision.

Mainstream applications of RMs are listed in [6.1.1](#). Not all types of RMs can be used for all indicated purposes.

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO/FDIS 33403](#)

<https://standards.iteh.ai/catalog/standards/iso/71b53ba4-41d1-49b0-95f8-bd7ee0a5a144/iso-fdis-33403>

Reference materials — Requirements and recommendations for use

1 Scope

This document describes good practice in using reference materials (RMs), and certified reference materials (CRMs) in particular, in measurement processes. These uses include:

- the assessment of precision and trueness of measurement methods;
- quality control;
- assigning values to materials;
- calibration;
- establishing conventional scales.

This document also relates key characteristics of various types of RMs to the different applications.

The preparation of RMs for calibration is also part of the scope of ISO 17034 and ISO Guide 35. The treatment in this document is limited to the fundamentals of small-scale preparation of RMs and the value assignment, as used by laboratories to calibrate their equipment. Larger scale production of such RMs, with the possible aim of distribution, is beyond the scope of this document. This type of activity is covered in ISO 17034 and ISO Guide 35.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO Guide 30, *Reference materials — Selected terms and definitions*

ISO/IEC Guide 99, *International vocabulary of metrology — Basic and general concepts and associated terms (VIM)*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO Guide 30 and ISO/IEC Guide 99 apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

4 Symbols

α	risk of error of the first type (type I error)
β	risk of error of the second type (type II error)
χ^2	chi-squared
d	measurement bias
k	coverage factor
s_w	standard deviation computed from repeat observations
σ_w	intralaboratory standard deviation
σ_{wo}	required intralaboratory standard deviation
$u()$	standard uncertainty of the parameter in parenthesis
$U()$	expanded uncertainty of the parameter in parenthesis
u_{CRM}	standard uncertainty associated with property value of the CRM
u_{meas}	standard uncertainty associated with value obtained by measuring the CRM
u_{prep}	uncertainty associated with the value obtained from preparation of a calibrant
x_{CRM}	value of a specified property of the CRM
x_{meas}	value obtained by measuring the CRM
x_{prep}	value obtained from preparation of a calibrant
\bar{x}	average of repeat observations

[ISO/FDIS 33403](https://standards.iteh.ai/Document/Preview/ISO/FDIS/33403)

5 Conventions

In this document, the following conventions are used:

A measurand is specified in such a way that there exists a unique, but unknowable, 'true value'.

All statistical methods used in this document are based on the following assumptions:

- a) The certified value is the best estimate of the true value of the property of the CRM.
- b) All variation, be it associated with the material (i.e. homogeneity) or the measurement process, is random and follows a normal probability distribution. The values of probabilities stated in this document assume normality. The probability may be different if there is deviation from normality.

Property values that are not certified values are considered to be unfit for use in metrological applications requiring a value assigned to the measurand, such as calibration, or the assignment of values to other materials.

Throughout this document, the law of propagation of uncertainty is used. Other methods of propagating uncertainties can be applied as well, and in some cases such alternative methods are required by the circumstances of the application. Further guidance on these matters is given in ISO/IEC Guide 98-3:2008 and its supplements.

6 RMs and their role in measurement

6.1 Common applications of RMs

6.1.1 RMs, and CRMs in particular, are widely used for the following purposes:


- method validation ([Clause 8](#) and [Clause 9](#));
- quality control of a measurement or measurement procedure ([Clause 8](#) and [Clause 9](#));
- establishing metrological traceability ([Clause 9](#), [Clause 10](#) and [Clause 11](#));
- calibration of equipment or a measurement procedure ([Clause 10](#));
- assigning values to other materials ([Clause 11](#));
- maintaining conventional scales ([Clause 12](#)).

[Figure 1](#) presents a schematic of how CRMs can be used in a measurement process. CRMs for calibration are often used to calibrate an analytical instrument. The data from the instrument calibration is usually used to set up a calibration curve that is used for the calculation of the measurement results. The uncertainty from the CRMs that were used for the calibration of the instrument will also be an uncertainty contribution to the uncertainty of the measurement results. Matrix CRMs are often also used for instrument calibration for measurement techniques that analyse solid samples, such as X-ray fluorescence for geological or mineralogical samples or laser ablation inductively coupled plasma mass spectrometry, as well as many other surface analysis techniques.

During method validation, matrix CRMs are usually used to evaluate the measurement trueness of the optimised method. This approach is especially applicable when the matrix of the CRM is a close match to the routine samples being analysed by the laboratory. It is also important to note that the same matrix CRM cannot be used to both calibrate the response of the measurement instrument and evaluate the measurement trueness during method validation.

ISO/FDIS 33403

<https://standards.iteh.ai/catalog/standards/iso/71b53ba4-41d1-49b0-95f8-bd7ee0a5a144/iso-fdis-33403>

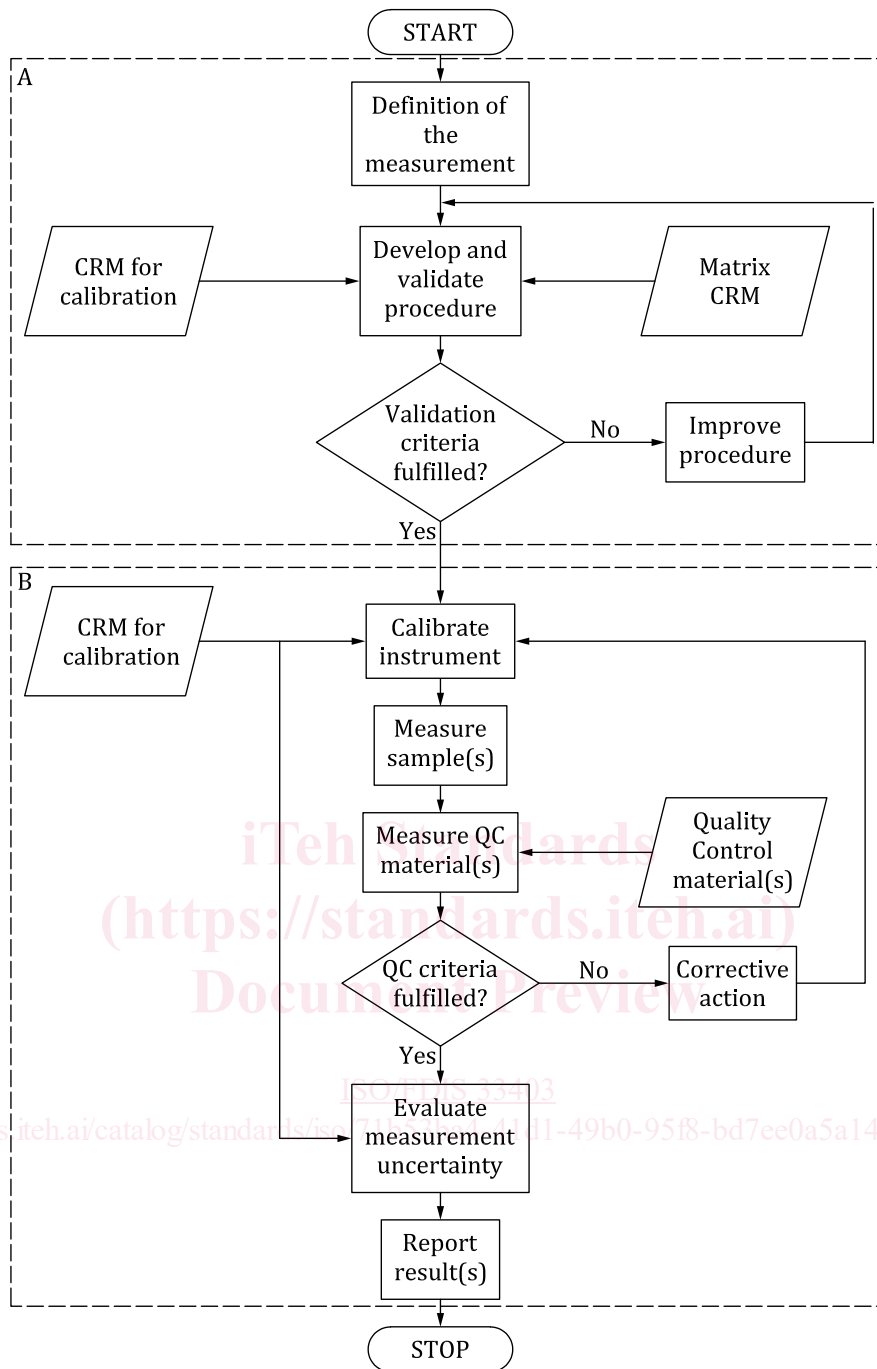

Key

- A procedure development and validation
- B routine measurement

Figure 1 — Schematic outline of a measurement and two possible uses of CRMs therein

6.1.2 Standards for the general requirements for the competence of laboratories, for example ISO/IEC 17025 and ISO 15189, require measurement results to be metrologically traceable and measurement equipment calibrated. Metrological traceability is a prerequisite for achieving comparable and compatible measurement results.

EXAMPLE A wine with a volume fraction of 12 % alcohol can be usefully compared with another wine with a volume fraction of 13,5 % alcohol.

6.1.3 It is usually taken for granted that measurement results, expressed in appropriate units, are comparable. In order to meet this implicit expectation of measurement data, laboratories should ensure that all equipment is properly calibrated using measurement standards, which in turn have been made metrologically traceable to the realization of the relevant unit. In many cases, this unit is part of the International System of Units (SI).

6.1.4 A summary list of key characteristics of RMs, cross-referenced to the common applications of RMs, is given in [Table 1](#).

Table 1 — Key characteristics of reference materials (RMs) and their relevance in common applications

	Assessment of precision	Bias assessment	Calibration/ conventional scales	Assigning values to other materials
Specification of the property of interest	Required	Required	Required	Required
Property value		Required	Required	Required
Stated uncertainty		Required	Required	Required
Specified level of homogeneity	Required	a	a	a
Specified level of stability	Required	a	a	a
Statement of metrological traceability		Required	Required	Required
Instructions for use	Required	Required	Required	Required
Expiry date of the certificate		Required	Required	Required
^a Uncertainty contribution included in the stated uncertainty associated with the property value.				

6.2 Property values

6.2.1 General

6.2.1.1 CRMs are characterized for one or more properties. These property values are accompanied by:

- a) a clear specification of the property concerned;
- b) an uncertainty statement;
- c) a statement of metrological traceability;
- d) a period of validity of the certificate.

The user should verify that all this information is available in an unambiguous form.

6.2.1.2 Indicative values should not be used for any of the uses of CRMs described in this document.

NOTE The terminology used in practice for indicative values is not always consistent with this document.

6.2.2 Specification of the property

6.2.2.1 The unambiguous specification of the property concerned assists greatly in deciding whether the CRM is appropriate for the user's intended application. The user of a CRM is responsible for assessing the suitability of the material for their own application.

EXAMPLE For trace elements in soil, it is important to specify whether it is the total content, content obtained by incomplete destruction (e.g. aqua regia), leachable content or a particular species containing the trace element.