



**International
Standard**

ISO 14085-3

**Aerospace series — Test methods
for hydraulic filter elements —**

**Part 3:
Filtration efficiency and retention
capacity**

*Série aérospatiale — Méthodes d'essais pour les éléments
filtrants hydrauliques —*

Partie 3: Efficacité de filtration et capacité de rétention

[ISO 14085-3:2024](https://standards.iteh.ai/standards/iso/14085-3:2024)

<https://standards.iteh.ai/catalog/standards/iso/76a110c9-825c-4e0d-9d51-5b038abb41a6/iso-14085-3-2024>

**Second edition
2024-05**

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

[ISO 14085-3:2024](https://standards.iteh.ai/catalog/standards/iso/76a110c9-825c-4e0d-9d51-5b038abb41a6/iso-14085-3-2024)

<https://standards.iteh.ai/catalog/standards/iso/76a110c9-825c-4e0d-9d51-5b038abb41a6/iso-14085-3-2024>



COPYRIGHT PROTECTED DOCUMENT

© ISO 2024

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	2
4 Symbols	4
5 Test procedure overview	5
6 Test apparatus	5
7 Instrument accuracy and allowable test condition variation	9
8 Test equipment validation	10
8.1 Steady flow filter test system validation.....	10
8.2 Cyclic flow filter test system validation.....	11
8.3 Contaminant injection system validation.....	12
9 Summary of information required prior to testing	13
10 Preliminary test preparation	13
10.1 Test filter assembly.....	13
10.2 Contaminant injection system.....	14
10.3 Steady flow filter test system.....	15
10.4 Cyclic flow filter test system.....	16
11 Filter element efficiency test	16
11.1 Steady flow test.....	16
11.2 Cyclic flow test.....	18
12 Calculation and data reporting	20
12.1 Filtration ratio and retention capacity.....	20
12.2 Calculation of stabilized particle counts for cyclic flow test.....	24
13 Identification statement (reference to this document)	28
Annex A (normative) Properties of test fluid to evaluate performance of hydraulic fluid systems filter elements	29
Annex B (informative) Test system design guidance	31
Bibliography	36

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO document should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

ISO draws attention to the possibility that the implementation of this document may involve the use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 20, *Aircraft and space vehicles*, Subcommittee SC 10, *Aerospace fluid systems and components*.

This second edition cancels and replaces the first edition (ISO 14085-3:2015), which has been technically revised.

The main changes are as follows:

- [Table 3](#) has been revised;
- [10.3.2](#) has been revised;
- Figure 4 has been converted to [Table 4](#) and [Table 5](#).

A list of all parts in the ISO 14085 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

In aerospace hydraulic fluid power systems, power is transmitted and controlled through a liquid under pressure. The liquid is both a lubricant and power-transmitting medium. The presence of solid contaminant particles in the liquid interferes with the ability of the hydraulic fluid to lubricate, and causes wear and malfunction of the components. The extent of contamination in the fluid has a direct bearing on the performance, reliability, and safety of the system, and should be controlled to levels that are considered appropriate for the system concerned.

Different principles are used to control the contamination level of the fluid by removing solid contaminant particles; one of them uses a filter element enclosed in a filter housing. The filter element is the porous device that performs the actual process of filtration. The complete assembly is designated as a filter.

The performance characteristics of a filter are a function of the filter element (its medium and geometry) and the housing (its general configuration and seal design). For a given filter, the actual performance is a function of the characteristics of the liquid (viscosity, temperature, conductivity, etc.), the particles in suspension (size, shape, hardness, etc.), and the flow conditions.

A standard multi-pass method for evaluating the performance of hydraulic fluid filter elements under steady state conditions has been developed and used for several years, and is referred to in several aircraft hydraulic systems specifications.

Most aircraft hydraulic systems are subjected to unsteady flow with flow cycles caused by such conditions as actuator movement. Such flow variations can have a significant impact on filter performance. The relative performance of hydraulic filters is compared in order to select the most appropriate filter. To ensure the reliability of such comparisons, it is necessary to perform testing with the same standard operating conditions.

This document describes two test methods and the equipment required to measure hydraulic filter element performance with multi-pass flow in both steady and cyclic conditions.

The influence of other stressful operating conditions, such as heat, cold, and vibration, are not measured with this procedure alone. The influence of such conditions is determined with pre-conditioning performed on the test filter element prior to efficiency testing (refer to ISO 14085-1 for descriptions of such tests and when they are applied).

The stabilized contamination level measured while testing with cyclic flow gives an indication of the average contamination level maintained by the filter in a dynamic operating system. The average system contamination level is important in establishing wear rates and reliability levels.

The measurements are made with precise control over the operating conditions, in particular the test fluid and test contaminant, to ensure repeatability and reproducibility. However, because the test parameters and test contaminant do not exactly replicate actual operating conditions which significantly differ from one system to another, the measurements cannot be expected to duplicate the actual performance in an operating system.

Aerospace series — Test methods for hydraulic filter elements —

Part 3: Filtration efficiency and retention capacity

1 Scope

This document describes two methods to measure in repeatable conditions the filtration efficiency of filter elements used in aviation and aerospace hydraulic fluid systems. It can be applied when evaluating the overall characteristics of a filter element according to ISO 14085-1, or separately.

Since the filtration efficiency of a filter element can change during its service life as it is clogging, this test method specifies its continuous measurement by using on-line particle counters with continuous injection of test contaminant and recirculation of particles not retained by the test filter element until the differential pressure across the element reaches a given final or “terminal” value.

This document allows the efficiency to be measured under both steady or cyclic flow conditions. It is also applicable to measuring the stabilized contamination levels that are produced by the filter element while testing with cyclic flow.

This document is not applicable to qualifying a filter element under replicate conditions of service; this can only be done by a specific test protocol developed for the purpose, including actual conditions of use, e.g. the operating fluid or contamination.

The test data resulting from application of this document can be used to compare the performance of aerospace hydraulic filter elements.

[ISO 14085-3:2024](https://standards.iteh.ai/catalog/standards/iso/76a110c9-825c-4e0d-9d51-5b038abb41a6/iso-14085-3-2024)

<https://standards.iteh.ai/catalog/standards/iso/76a110c9-825c-4e0d-9d51-5b038abb41a6/iso-14085-3-2024>

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 2942, *Hydraulic fluid power — Filter elements — Verification of fabrication integrity and determination of the first bubble point*

ISO 3968, *Hydraulic fluid power — Filters — Evaluation of differential pressure versus flow*

ISO 4021, *Hydraulic fluid power — Particulate contamination analysis — Extraction of fluid samples from lines of an operating system*

ISO 4405, *Hydraulic fluid power — Fluid contamination — Determination of particulate contamination by the gravimetric method*

ISO 5598, *Fluid power systems and components — Vocabulary*

ISO 11171, *Hydraulic fluid power — Calibration of automatic particle counters for liquids*

ISO 11218, *Aerospace — Cleanliness classification for hydraulic fluids*

ISO 11943, *Hydraulic fluid power — Online automatic particle-counting systems for liquids — Methods of calibration and validation*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 5598 and the following apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

3.1

contaminant mass injected

mass of a specific particulate contaminant injected into the test circuit to obtain the terminal differential pressure

3.2

cyclic flow


change of flow from the specified rated flow rate to 25 % of the rated flow rate at a specified frequency and waveform

3.3

differential pressure

Δp
difference between the inlet and outlet pressures of the component under test, as measured under specified conditions


Note 1 to entry: See [Figure 1](#) and [Figure 2](#) for graphical depiction of *differential pressure* (3.3) terms.

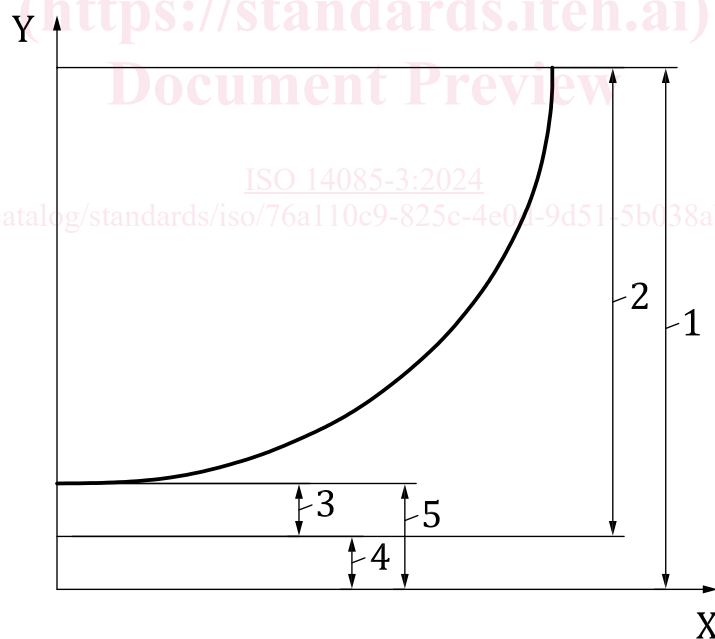

Key

X	test time or mass injected	3	clean element differential pressure
Y	differential pressure	4	housing differential pressure
1	final assembly (end of test) differential pressure	5	clean assembly differential pressure
2	terminal element differential pressure		

Figure 1 — Differential pressure conventions for multi-pass test with steady flow

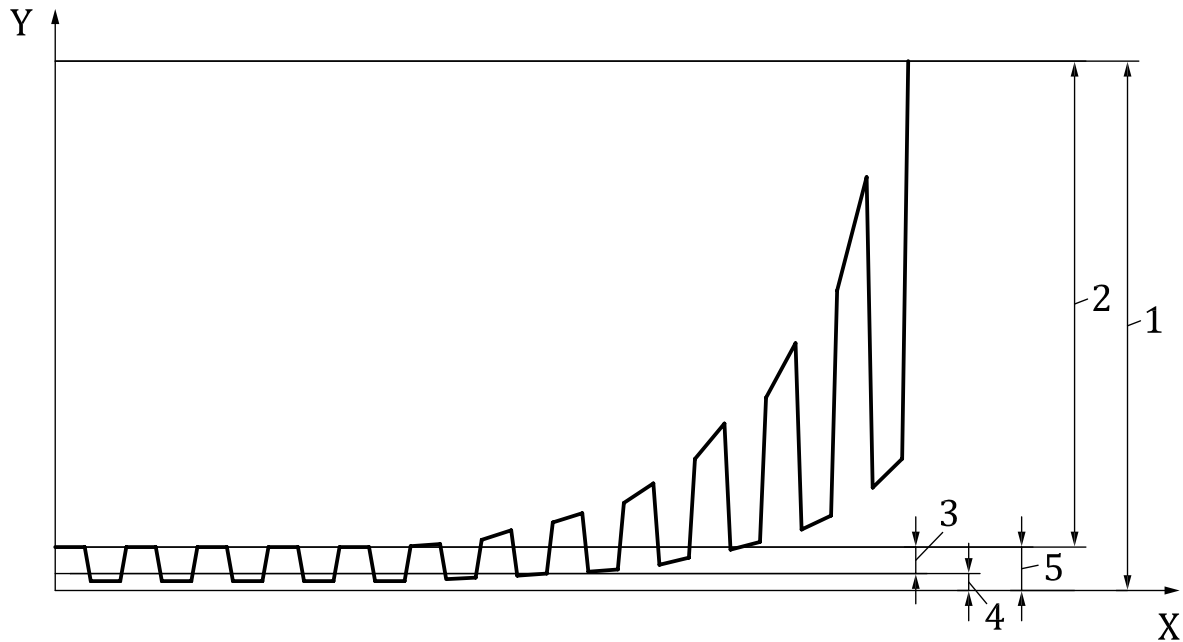

Key

X	test time or mass injected	3	clean element differential pressure at test flow rate (q_f)
Y	differential pressure	4	housing differential pressure at test flow rate (q_f)
1	final assembly (end of test) differential pressure	5	clean assembly differential pressure at test flow rate (q_f)
2	terminal element differential pressure at test flow rate (q_f)		

Figure 2 — Differential pressure conventions for multi-pass test with cyclic flow

3.3.1

clean assembly differential pressure

difference between the tested component inlet and outlet pressure as measured with a clean filter housing containing a clean filter element

3.3.2

clean element differential pressure

differential pressure (3.3) of the clean element calculated as the difference between the *clean assembly differential pressure (3.3.1)* and the *housing differential pressure (3.3.4)*

3.3.3

final assembly differential pressure

assembly differential pressure (3.3) at end of test equal to sum of housing plus *terminal element differential pressures (3.3.5)*

3.3.4

housing differential pressure

differential pressure (3.3) of the filter housing without an element

3.3.5

terminal element differential pressure

maximum *differential pressure (3.3)* across the filter element as designated by the manufacturer or specification to limit useful performance

3.4

filtration ratio

ratio of the number of particles larger than a specified size per unit volume in the influent fluid to the number of particles larger than the same size per unit volume in the effluent fluid

Note 1 to entry: For steady flow testing, the filtration ratios are designated with the Greek letter beta, β .

Note 2 to entry: For *cyclic flow* (3.2) testing, the filtration ratios are designated with the Greek letter sigma, σ .

3.5

free-flow dummy element

duplicate test filter element with its media layers removed to replicate the flow pattern in the housing generated by the test filter element

3.6

rest conductivity

electrical conductivity at the initial instant of current measurement after a DC voltage is impressed between electrodes

Note 1 to entry: It is the reciprocal of the resistance of uncharged fluid in the absence of ionic depletion or polarization.

3.7

retention capacity

mass of specific particulate contaminant effectively retained by the filter element when *terminal element differential pressure* (3.3.5) is reached

4 Symbols

Symbol	Unit	Description or explanation
$\bar{A}_{u,x}$	particles per millilitre	Overall average upstream count greater than size, x
$\bar{A}_{d,x}$	particles per millilitre	Overall average downstream count greater than size, x
\bar{c}_b	mg/l	Average base upstream gravimetric level
c_b	mg/l	Desired base upstream gravimetric level
\bar{c}_i	mg/l	Average injection gravimetric level
c_i'	mg/l	Desired injection gravimetric level
c_{80}	mg/l	Test reservoir gravimetric level at 80 % assembly Δp
m	G	Mass of contaminant needed for injection
m_e	G	Estimated filter element capacity (mass injected)
m_i	G	Contaminant mass injected
m_p	G	Contaminant mass injected at element differential pressure
m_R	G	Retained capacity
n	None	Number of counts in specific time period
$N_{u,x,j}$	particles per millilitre	Number of upstream particles greater than size, x , at count, j
$N_{d,x,j}$	particles per millilitre	Number of downstream particles greater than size, x , at count, j
$\bar{N}_{u,x,t}$	particles per millilitre	Average upstream count greater than size, x , at time interval, t
$\bar{N}_{d,x,t}$	particles per millilitre	Average downstream count greater than size, x , at time interval, t
Δp	Pa or kPa (bar)	Differential pressure
Δp_f	Pa or kPa (bar)	Final assembly differential pressure

Symbol	Unit	Description or explanation
Δp_n	Pa or kPa (bar)	Net assembly differential pressure
$\Delta p_{2,5\%}$	Pa or kPa (bar)	Assembly differential pressure after increase of 2,5 % net Δp
$\Delta p_{80\%}$	Pa or kPa (bar)	Assembly differential pressure after increase of 80 % net Δp
\bar{q}_f	l/min	Average filter test flow rate
q_d	l/min	Discarded downstream sample flow rate
q_f	l/min	Filter rated flow (maximum flow for cyclic conditions)
q_i'	l/min	Desired injection flow rate
\bar{q}_i	l/min	Average injection flow rate
q_u	l/min	Discarded upstream sample flow rate
t	min	Test time
t'	min	Predicted test time
t_f	min	Final test time
t_i	min	Total injection time
t_p	min	Test time at element differential pressure
$t_{2,5\%}$	min	Test time at beginning of 2,5 % stabilization period
$t_{80\%}$	min	Test time at beginning of 80 % stabilization period
V_{if}	l	Final measured injection system volume
V_{ii}	l	Initial measured injection system volume
V_{min}	l	Minimum required operating injection system volume
V_{tf}	l	Final measured filter test system volume
V_v	l	Minimum validated injection system volume
x, x_1, x_2	$\mu\text{m(c)}$	Particle sizes
β_x	None	Filtration ratio at particle size, x (steady flow)
$\beta_{x,t}$	None	Filtration ratio at particle size, x , and time interval, t (steady flow)
$\bar{\beta}_x$	None	Average filtration ratio at particle size x (steady flow)
σ_x	None	Filtration ratio at particle size, x (cyclic flow)
$\sigma_{x,t}$	None	Filtration ratio at particle size, x , and time interval, t (cyclic flow)
$\bar{\sigma}_x$	None	Average filtration ratio at particle size, x (cyclic flow)

5 Test procedure overview

- 5.1 Set up and maintain apparatus in accordance with [Clause 6](#) and [Clause 7](#).
- 5.2 Validate equipment in accordance with [Clause 8](#).
- 5.3 Run all tests in accordance with [Clauses 9, 10](#), and [11](#).
- 5.4 Analyse and present data from [Clause 11](#) in accordance with [Clause 12](#).

6 Test apparatus

6.1 Suitable timer

6.2 Sample bottles, use applicable sample bottles containing less than 100 particles greater than 6 $\mu\text{m(c)}$ per millilitre of bottle volume, as qualified in accordance with ISO 3722, to collect samples for gravimetric analyses.

6.3 Membrane filters and associated equipment, suitable for conducting gravimetric contamination analysis in accordance with ISO 4405.

6.4 Test contaminant, use ISO fine test dust (ISO FTD), grade A2 in accordance with ISO 12103-1, dried at 110 °C to 150 °C for not less than 1 h for quantities less than 200 g.

Ensure that the ISO FTD used conforms to all the requirements of ISO 12103-1 grade A2, especially the volume particle size distribution shown in ISO 12103-1:2024, Table 2.

NOTE If the total quantity of ISO FTD needed is greater than 200 g, batches not exceeding 200 g can be prepared to make up the amount required.

For use in the test system the test dust should be mixed into the test fluid, mechanically agitated, then dispersed ultrasonically in an ultrasonic bath that has a power density of 3 000 W/m² to 10 000 W/m² provided it has been demonstrated that ultrasonic energy used does not affect the fluid viscosity.

6.5 Test fluid, petroleum base test fluid which shall have the properties as detailed in [Annex A](#).

Another standard test fluid shall be used provided there is agreement between parties. Only filter test results obtained with the same fluid shall be compared.

The temperature of the test fluid, during the test, shall be controlled at a value to result in a test fluid kinematic viscosity of 15 mm²/s ± 1 mm²/s.

NOTE 1 The use of this hydraulic fluid ensures greater reproducibility of results and is based upon current practices, other accepted filter standards, and its world-wide availability.

NOTE 2 The addition of an anti-static agent to this test fluid can affect the test results.

6.6 Particle counting systems

6.6.1 An online automatic particle counting system, in accordance with ISO 11943, shall be used to determine the number and size distribution of the contaminant particles in the fluid. An online dilution system may be required to ensure that the particulate concentration in the fluid sampled by the automatic particle counters does not exceed the saturation limits specified by the automatic particle counter manufacturer. <https://standards.iteh.ai/catalog/standards/iso/76a110c9-825c-4e0d-9d51-5b038abb41a6/iso-14085-3-2024>

The automatic particle counters, including the on-line dilution system, if applicable, should be validated for on-line counting in accordance with ISO 11943.

6.6.2 A turbulent sampling means, in accordance with ISO 4021, shall be located upstream and downstream of the test filter element in order to provide fluid sample flow to the automatic particle counters. The design of the sampling system shall be such as to minimize lag time in fluid flow to the automatic particle counters. The portion of the sampling flow not passing through the automatic particle counters can be returned to the filter element test circuit reservoir via a by-pass line. Flow through the automatic particle counters can also be returned to the filter element test circuit reservoir provided it has not been diluted, or it can be discarded. Do not interrupt sample flow during the test.

6.6.3 Automatic particle counters shall be calibrated in accordance with ISO 11171 for the appropriate particle sizes. Use the recommended particle sizes given in [Table 2](#) unless otherwise agreed.

6.7 Test housing and free flow dummy element

6.7.1 The service filter housing shall be used whenever possible; and it shall be installed in a normal service attitude. If this housing contains a by-pass valve, it shall be blocked and tested for zero leakage at twice the normal cracking pressure.