

ISO/FDIS 6508-1

ISO/TC 164/SC 3

~~Date: 2023-01-10~~

~~ISO/DIS 6508-1:2022(E)~~

~~ISO/TC 164/SC 3/WG~~

Secretariat: DIN

~~Date: 2023-08-02~~

Metallic materials — Rockwell hardness test —

**Part 1:
Test method**

Matériaux métalliques — Essai de dureté Rockwell —

Partie 1: Méthode d'essai

iTeh Standards
(<https://standards.iteh.ai>)
Document Preview

ISO 6508-1

<https://standards.iteh.ai/catalog/standards/sist/8ba64bea-7af0-4ef5-a019-5835dfd17b34/iso-6508-1>

FDIS stage

~~Edited DIS -
MUST BE USED
FOR FINAL
DRAFT~~

© ISO ~~2022~~ 2023

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: + 41 22 749 01 11

Fax: +41 22 749 09 47

~~Email~~E-mail: copyright@iso.org
Website: www.iso.org

Published in Switzerland

iTeh Standards (<https://standards.iteh.ai>) Document Preview

[ISO 6508-1](#)

<https://standards.iteh.ai/catalog/standards/sist/8ba64bea-7af0-4ef5-a039-5835dfd17b34/iso-6508-1>

Contents

Forewordiv

1 Scope1

2 Normative references.....1

3 Terms and definitions1

4 Symbols, abbreviated terms and designations1

5 Rockwell hardness.....3

6 Testing machine5

7 Test piece.....5

8 Procedure.....6

9 Uncertainty of the results8

10 Test report8

11 Conversions to other hardness scales or tensile strength values8

Annex A (normative) Special HR30T_{Sm} and HR15T_{Sm} test for thin products.....9

Annex B (normative) Minimum thickness of the test piece in relation to the Rockwell hardness 10

Annex C (normative) Corrections to be added to Rockwell hardness values obtained on convex cylindrical surfaces 16

Annex D (normative) Corrections to be added to Rockwell hardness C scale values obtained on spherical test surfaces of various diameters..... 19

Annex E (normative) Daily verification procedure.....20

Annex F (normative) Inspection of diamond indenters.....23

Annex G (informative) Uncertainty of the measured hardness values.....24

Annex H (informative) CCM — Working group on hardness.....29

Annex I (informative) Rockwell hardness measurement traceability30

Bibliography34

~~Edited DIS~~
~~MUST BE USED~~
~~FOR FINAL~~
~~DRAFT~~

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

~~Attention is drawn~~ ISO draws attention to the possibility that ~~some of the elements~~ implementation of this document may ~~be involve~~ the ~~subject~~ use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights. ~~Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see).~~

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 164, *Mechanical testing of metals*, Subcommittee SC 3, *Hardness testing*, in collaboration with the European Committee for Standardization (CEN) Technical Committee CEN/TC 451459, *ECISS - European Committee for Iron and Steel Standardization, SC 1, Test methods for steel (other than chemical analysis)*, in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

This fifth edition cancels and replaces the fourth edition (ISO 6508-1:2016), which has been technically revised.

The main changes are as follows:

- ~~removal of note related to the use of tungsten and steel ball indenters (Clause 1 (Clause 1))~~;
- removal of the year from the Normative References specified and various places throughout the body of the standard ~~(Clause 2 (Clause 2))~~;
- ~~addition~~ addition of ~~Clause 3 (Clause 3)~~, Terms and definitions;

iv

4

© ISO 2022 – All rights reserved

© ISO 2023 – All rights reserved

- ~~Added~~ additional information for the use of single-piece spherically tipped indenters (5.3 ~~Note~~NOTE 1);
- ~~Added~~ the table reference and table title (7.4(7.4));
- ~~Modified~~modified the uncertainty of the results section to only provide a single reference for the determination of uncertainty (Clause 8-(Clause 9));
- ~~modified Annex C~~Modified Annex C, Uncertainty of the measured hardness values, to remove the “procedure without bias (M2)” method for determining uncertainty (Annex G(Annex G)-).

A list of all parts in the ISO 6508 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user’s national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

iTech Standards
(<https://standards.iteh.ai>)
Document Preview

ISO 6508-1

<https://standards.iteh.ai/catalog/standards/sist/8ba64bea-7af0-4ef5-a039-5835dfd17b34/iso-6508-1>

~~Edited DIS~~
~~MUST BE USED~~
~~FOR FINAL~~
~~DRAFT~~

Metallic materials — Rockwell hardness test —

Part 1: Test method

1 Scope

This document specifies the method for Rockwell regular and Rockwell superficial hardness tests for scales A, B, C, D, E, F, G, H, K, 15N, 30N, 45N, 15T, 30T, and 45T for metallic materials and is applicable to stationary and portable hardness testing machines.

For specific materials and/or products, other specific International Standards apply (e.g. ISO 3738-1 and ISO 4498).

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 6508-2¹, *Metallic materials — Rockwell hardness test — Part 2: Verification and calibration of testing machines and indenters*

ISO 6508-3, *Metallic materials — Rockwell hardness test — Part 3: Calibration of reference blocks*

3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

4 Symbols, abbreviated terms and designations

According to [Table 1](#), [Table 2](#), [Table 3](#), and [Figure 1](#).

Table 1 — Rockwell ~~Regular~~ regular scales

Rockwell Regular hardness scale	Hardness symbol Unit	Type of indenter	Preliminary force F_0	Total force F	Scaling Constant S	Full Range Constant N	Applicable range of application (Rockwell Regular hardness scales)
A	HRA	Diamond cone	98,07 N	588,4 N	0,002 m m	100	20 HRA to 95 HRA

¹ Fourth edition under preparation. Stage at the time of publication: ISO/FDIS 6508-2:2023.

ISO/FDIS 6508-1:2023(E)

Rockwell Regular hardness scale	Hardness symbol Unit	Type of indenter	Preliminary force F_0	Total force F	Scaling Constant S	Full Range Constant N	Applicable range of application (Rockwell Regular hardness scales)
B	HRBW	Ball 1,587 5 mm	98,07 N	980,7 N	0,002 m	130	10 HRBW to 100 HRBW
C	HRC	Diamond cone	98,07 N	1,471 k N	0,002 m	100	20 HRC ^a to 70 HRC
D	HRD	Diamond cone	98,07 N	980,7 N	0,002 m	100	40 HRD to 77 HRD
E	HREW	Ball 3,175 mm	98,07 N	980,7 N	0,002 m	130	70 HREW to 100 HREW
F	HRFW	Ball 1,587 5 mm	98,07 N	588,4 N	0,002 m	130	60 HRFW to 100 HRFW
G	HRGW	Ball 1,587 5 mm	98,07 N	1,471 k N	0,002 m	130	30 HRGW to 94 HRGW
H	HRHW	Ball 3,175 mm	98,07 N	588,4 N	0,002 m	130	80 HRHW to 100 HRHW
K	HRKW	Ball 3,175 mm	98,07 N	1,471 k N	0,002 m	130	40 HRKW to 100 HRKW

^a The applicable range of application can be extended to 10 HRC if the surfaces of the diamond cone and spherical tip are polished for a penetration depth of at least 0,4 mm.

Table 2 — Rockwell Superficial scales

Rockwell Superficial hardness scale	Hardness symbol Unit	Type of indenter	Preliminary force F_0	Total force F	Scaling Constant S	Full Range Constant N	Applicable range of application (Rockwell Superficial hardness scales)
15N	HR15N	Diamond cone	29,42 N	147,1 N	0,001 m	100	70 HR15N to 94 HR15N
30N	HR30N	Diamond cone	29,42 N	294,2 N	0,001 m	100	42 HR30N to 86 HR30N
45N	HR45N	Diamond cone	29,42 N	441,3 N	0,001 m	100	20 HR45N to 77 HR45N
15T	HR15TW	Ball 1,587 5 mm	29,42 N	147,1 N	0,001 m	100	67 HR15TW to 93 HR15TW
30T	HR30TW	Ball 1,587 5 mm	29,42 N	294,2 N	0,001 m	100	29 HR30TW to 82 HR30TW
45T	HR45TW	Ball 1,587 5 mm	29,42 N	441,3 N	0,001 m	100	10 HR45TW to 72 HR45TW

Scales using indenter balls with diameter 6,350 mm and 12,70 mm may also be used, if specified in the product specification or by special agreement. See ASTM E18 [5] for additional scales using these ball sizes.

NOTE 1 For certain materials, it is possible that the applicable range of application might be narrower than those indicated.

NOTE 2 The numbers representing the test forces were originally based on units of kgf. For example, the total test force of 30 kgf has been converted to 294,2 N.


Table 3 — Symbols and abbreviated terms

Symbol/ Abbreviated abbreviated term	Definition	Unit
F_0	Preliminary test force	N
F_1	Additional test force (total force minus preliminary force)	N
F	Total test force	N
S	Scaling constant, specific to the scale	mm
N	Full range constant, specific to the scale	-
h	Permanent depth of indentation under preliminary test force after removal of additional test force (permanent indentation depth)	mm
HRA HRC HRD	Rockwell Regular regular hardness $= 100 - \frac{h}{0,002}$	
HRBW HREW HRFW HRGW HRHW HRKW	Rockwell Regular regular hardness $= 130 - \frac{h}{0,002}$	
HRN HRTW	Rockwell Superficial superficial hardness $= 100 - \frac{h}{0,001}$	


5 Rockwell hardness

5.1 The following is an example of the designation of Rockwell hardness.

EXAMPLE 70 HR30TW, where:

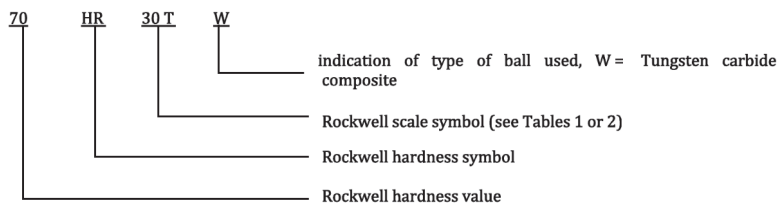


ISO/FDIS 6508-1:2023(E)

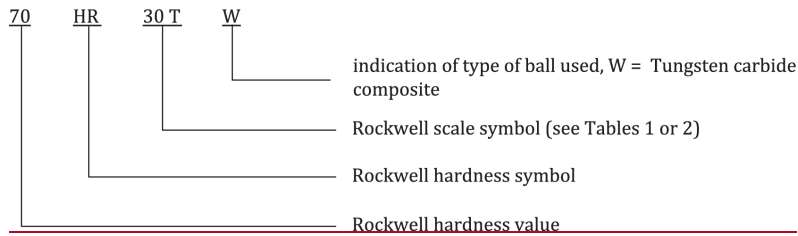


NOTE 1 Previous versions of this part of ISO 6508 document allowed the use of steel indenter balls, which required the suffix S.

NOTE 2 For the HR30T_Sm and HR15T_Sm scales specified in Annex A, a capital S and a lower-case m are used indicating the use of steel indenter balls and a diamond spot specimen holder.

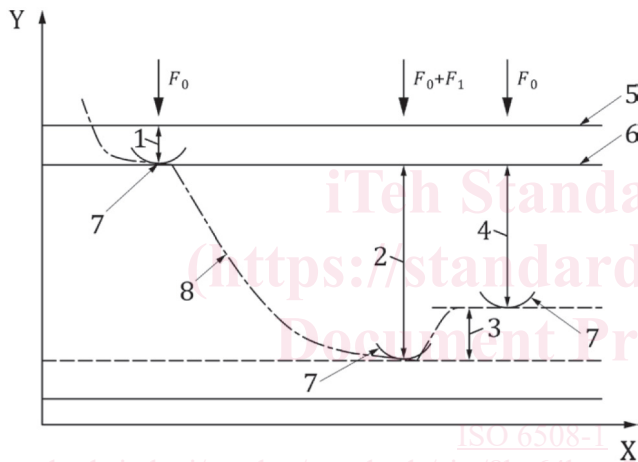

<https://standards.iteh.ai/catalog/standards/sist/8ba64bea-7af0-4ef5-a039-5835dfd17b34/iso-6508-1>

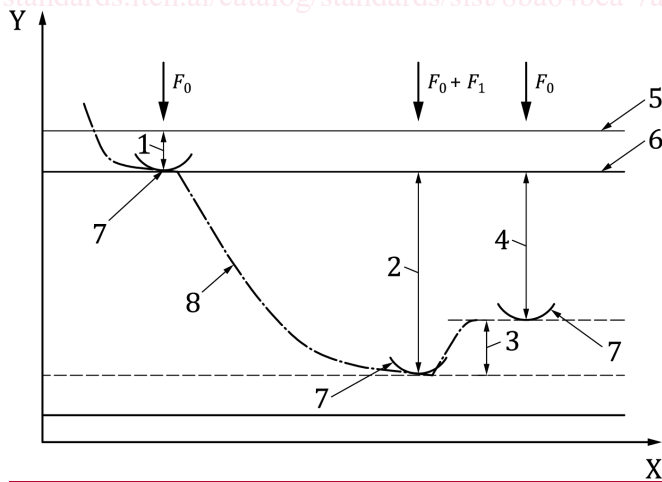

Key

X time

4 permanent indentation depth, *h*

Y	indenter position	5	surface of specimen
1	indentation depth by preliminary force, F_0	6	reference plane for measurement
2	indentation depth by additional test force, F_1	7	position of indenter
3	elastic recovery just after removal of additional test force, F_1	8	indentation depth vs. time curve

Figure 1 — Rockwell principle diagram

5.2 Principle:

An indenter of specified size, shape, and material is forced into the surface of a test specimen under two force levels using the specific conditions specified in Clause 8 Clause 7. The specified preliminary force is applied and the initial indentation depth is measured, followed by the application and removal of a specified additional force, returning to the preliminary force. The final indentation depth is then measured and the Rockwell hardness value (H) is derived from the difference, h , in the final and initial indentation depths and the two constants N and S (see Figure 1, Table 1 Figure 1, Table 1, and Table 2 Table 2) as shown in Formula (1) Formula (1):

$$H = N - \frac{h}{S} \quad (1)$$

6 Testing machine

5.6.1 Testing machine, shall be capable of applying the test forces for some or all of the Rockwell hardness scales as shown in Table 1 Table 1 and Table 2 Table 2, performing the procedure specified in Clause 8 Clause 7, and complying with all of the requirements specified in ISO 6508-2.

5.6.2 Spheroconical diamond indenter, shall be in accordance with ISO 6508-2, with an included angle of 120° and radius of curvature at the tip of 0,2 mm. Diamond indenters shall be certified for use for either

- only the regular Rockwell diamond scales,
- only the superficial Rockwell diamond scales, or
- both the regular and the superficial Rockwell diamond scales.

5.6.3 Ball indenter, shall be tungsten carbide composite in accordance with ISO 6508-2, with a diameter of 1,587 5 mm or 3,175 mm (see NOTE 1 and NOTE 2).

NOTE 1 Ball indenters normally consist of a spherical ball and a separate appropriately designed holder. Single-piece spherically tipped indenters are allowed, provided that the surface of the indenter that makes contact with the test piece meets the size, shape, finish, and hardness requirements for the calibration and verification of the ball indenter as specified in ISO 6508-2, and meets the performance requirements for the indirect verification of the ball holder assembly as specified in ISO 6508-2.

NOTE 2 Attention is drawn to the fact that the use of tungsten carbide composite for ball indenters is the standard type of Rockwell indenter ball. Steel indenter balls can only be used when performing Rockwell HR30Tsm and HR15Tsm tests according to Annex A Annex A.

7 Test piece

6.7.1 The test shall be carried out on a surface which is smooth and even, free from oxide scale, foreign matter and, in particular, completely free from lubricants, unless specified otherwise in product or materials standards.

ISO/FDIS 6508-1:2023(E)

An exception is made for reactive metals, such as titanium, which might adhere to the indenter. In such situations, a suitable lubricant such as kerosene may be used. The use of a lubricant shall be reported on the test report.

67.2 Preparation shall be carried out in such a way that any alteration of the surface hardness due to excessive heating or cold-working for example, is minimized.

This shall be taken into account, particularly in the case of low-depth indentations.

67.3 The thickness of the test piece, or of the layer under test (minimum values are given in [Annex B](#)), shall be at least 10 times the permanent indentation depth for diamond indenters and 15 times the permanent indentation depth for ball indenters, unless it can be demonstrated that the use of a thinner test piece does not affect the measured hardness value.

In general, no deformation should be visible on the back of the test piece after the test, although not all such marking is indicative of a bad test.

See [Annex A](#) for special requirements for testing very thin sheet metal using the HR30T_{Sm} and HR15T_{Sm} scales.

67.4 For tests on convex cylindrical surfaces and spherical surfaces, see [8.11](#).

8 Procedure

78.1 This part of ISO 6508 document has been developed with a laboratory temperature requirement of 10 °C to 35 °C.

For environments outside the stated requirement, it is the responsibility of the testing laboratory to assess the impact on testing data produced with testing machines operated in such environments. When testing is performed outside the recommended temperature limits of 10 °C to 35 °C, the temperature shall be recorded and reported.

NOTE If significant temperature gradients are present during testing and/or calibration, measurement uncertainty can increase and out of tolerance conditions can occur.

78.2 The daily verification specified in [Annex E](#) shall be performed before the first test of each day for each scale to be used.

The condition of diamond indenters should be checked according to [Annex F](#).

78.3 After each change, or removal and replacement, of the indenter, indenter ball, or test piece support, perform at least two tests and discard the results, then determine that the indenter and the test piece support are correctly mounted in the machine by performing the daily verification process specified in [Annex E](#).

78.4 The diamond or ball indenter shall have been the indenter used during the last indirect verification.

If the indenter was not used during the indirect verification and is being used for the first time, it shall be verified in accordance with the daily verification given in [Annex E](#) using at least two test blocks (one from the low and high ranges as specified by the table in ISO 6508-2 titled "Hardness ranges for different scales");—², Table 1) for each Rockwell scale that is normally used. This does not apply to replacing a ball.

78.5 The test piece shall be placed on a rigid support and supported in such a manner that the surface to be indented is in a plane normal to the axis of the indenter and the line of the indenting force, as well as to avoid a displacement of the test piece.

² Fourth edition under preparation. Stage at the time of publication: ISO/FDIS 6508-2:2023.