

ISO/DTR 9464:2023(E)

Second edition

2023-03-16xx

**Guidelines for the use of ISO 5167:2022**

*Lignes directrices pour l'utilisation de l'ISO 5167:2022*

**Style Definition:** Heading 1: Indent: Left: 0 pt, First line: 0 pt, Tab stops: Not at 21.6 pt

**Style Definition:** Heading 2: Font: Bold, Tab stops: Not at 18 pt

**Style Definition:** Heading 3: Font: Bold

**Style Definition:** Heading 4: Font: Bold

**Style Definition:** Heading 5: Font: Bold

**Style Definition:** Heading 6: Font: Bold

**Style Definition:** ANNEX

**Style Definition:** AMEND Terms Heading: Font: Bold

**Style Definition:** AMEND Heading 1 Unnumbered: Font: Bold

**Formatted:** Italian (Italy)

**Formatted:** Italian (Italy)

**Formatted:** Font: Not Bold

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

ISO/DTR 9464

<https://standards.iteh.ai/catalog/standards/sist/80993c42-eef5-41d1-b8c5-47bbb5c87216/iso-dtr-9464>

© ISO 2023

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO Copyright Office

CP 401 • CH-1214 Vernier, Geneva

Phone: + 41 22 749 01 11

Email: [copyright@iso.org](mailto:copyright@iso.org)

Website: [www.iso.org](http://www.iso.org)

Published in Switzerland.

Formatted: Pattern: Clear

Formatted: Pattern: Clear

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

ISO/DTR 9464

<https://standards.iteh.ai/catalog/standards/sist/80993c42-eef5-41d1-b8c5-47bbb5c87216/iso-dtr-9464>

<b>Contents</b>	<b>Page</b>
<b>Foreword</b> .....	<b>iv</b>
<b>Introduction</b> .....	<b>v</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>2</b>
<b>4 How the structure of this guide relates to ISO 5167:2022 (all parts)</b> .....	<b>2</b>
<b>5 Guidance on the use of ISO 5167:2022 (all parts)</b> .....	<b>2</b>
<b>5.1 Guidance specific to the use of ISO 5167-1:2022</b> .....	<b>2</b>
<b>5.2 Guidance specific to the use of ISO 5167-2:2022</b> .....	<b>8</b>
<b>5.3 Guidance specific to the use of ISO 5167-3:2022</b> .....	<b>24</b>
<b>5.4 Guidance specific to the use of ISO 5167-4:2022</b> .....	<b>26</b>
<b>6 Information of a general nature relevant to the application of ISO 5167:2022 (all parts)</b> .....	<b>26</b>
<b>6.1 Secondary instrumentation</b> .....	<b>26</b>
<b>6.2 Measurement of pressure and differential pressure</b> .....	<b>28</b>
<b>6.3 Measurement of temperature</b> .....	<b>30</b>
<b>6.4 Determination of density</b> .....	<b>34</b>
<b>6.5 Electrical supply and electrical installations</b> .....	<b>39</b>
<b>Annex A (informative) Principles of measurement and computation</b> .....	<b>40</b>
<b>Annex B (informative) Computation of compressibility factor for natural gases</b> .....	<b>56</b>
<b>Annex C (informative) Orifice plate assembly</b> .....	<b>57</b>
<b>Bibliography</b> .....	<b>66</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

~~International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.~~

~~The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.~~

~~In exceptional circumstances, when a technical committee has collected data of a different kind from that which is normally published as an International Standard ("state of the art", for example), it may decide by a simple majority vote of its participating members to publish a Technical Report. A Technical Report is entirely informative in nature and does not have to be reviewed until the data it provides are considered to be no longer valid or useful.~~

~~Attention is drawn to the procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO document should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).~~

~~ISO draws attention to the possibility that some of the elements implementation of this document may involve the subject use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights, in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at [www.iso.org/patents](http://www.iso.org/patents). ISO shall not be held responsible for identifying any or all such patent rights.~~

~~Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.~~

~~For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).~~

ISO/TR 9464 was prepared by Technical Committee ISO/TC 30, *Measurement of fluid flow in closed conduits*, Subcommittee SC 2, *Pressure differential devices*.

This third edition cancels and replaces the second edition (ISO/TR 9464:2008), which has been technically revised.

The main changes are as follows:

— this document has been revised to be consistent with ISO 5167:2022.

ISO/DTR 9464:2023(E)

- this document is consistent with ISO/IEC Guide 98-3;
- the subclause on pressure transmitters has been updated.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at [www.iso.org/members.html](http://www.iso.org/members.html).

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

ISO/DTR 9464

<https://standards.iteh.ai/catalog/standards/sist/80993c42-eef5-41d1-b8c5-47bbb5c87216/iso-dtr-9464>

ISO/DTR 9464:2023(E)

## Introduction

The objective of this ~~Technical Report document~~ is to assist users of ISO 5167, which was published in 2022 in six parts. Guidance on particular clauses of ISO 5167:2022 is given.

Some clauses of ISO 5167:2022 (~~parts 1 to 6~~) ~~series~~ are not commented upon and the corresponding clause numbers are therefore omitted from this ~~Technical Report document~~, except when it has been thought to be useful to keep a continuous numbering of paragraphs.

iTeh STANDARD PREVIEW  
(standards.iteh.ai)

ISO/DTR 9464

<https://standards.iteh.ai/catalog/standards/sist/80993c42-eef5-41d1-b8c5-47bbb5c87216/iso-dtr-9464>

## Guidelines for the use of ISO 5167:2022

### 1 Scope

The objective of this ~~Technical Report document~~ is to provide guidance on the use of ~~ISO 5167:2022 (all parts), series, ISO 5167:2022~~ is an International Standard for flow measurement based on the differential pressure generated by a constriction introduced into a circular conduit (see ~~ISO 5167-1:2022, 5.1~~). It presents a set of rules and requirements based on theory and experimental work undertaken in the field of flow measurement.

For a more detailed description of the scope, reference ~~should be~~ made to ~~ISO 5167-1:2022, Clause 1~~. Definitions and symbols applicable to this Technical Report are given in ~~ISO 5167-1:2022, Clauses 3 and 4~~.

Neither ~~ISO 5167-1:2022~~ nor this ~~Technical Report document~~ give detailed theoretical background, for which reference ~~should be~~ made to any general textbook on fluid flow.

### 2 Normative references

The following ~~referenced~~ documents are ~~indispensable for referred to in the application text in such a way that some or all of their content constitutes requirements~~ of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

~~<std>ISO 2186, Fluid flow in closed conduits — Connections for pressure signal transmissions between primary and secondary elements</std>~~

~~<std>ISO/TR 3313:2018, Measurement of fluid flow in closed conduits — Guidelines on the effects of flow pulsations on flow measurement instruments</std>~~

~~<std>ISO 4006, Measurement of fluid flow in closed conduits — Vocabulary and symbols</std>~~

~~<std>ISO 5167-1:2022, Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full — Part 1: General principles and requirements</std>~~

~~<std>ISO 5167-2:2022, Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full — Part 2: Orifice plates</std>~~

~~<std>ISO 5167-3:2022, Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full — Part 3: Nozzles and Venturi nozzles</std>~~

~~<std>ISO 5167-4:2022, Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full — Part 4: Venturi tubes</std>~~

~~<std>ISO 5167-5:2022, Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full — Part 5: Cone meters</std>~~

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Adjust space between Latin and Asian text, Adjust space between Asian text and numbers

~~<std>ISO 5167-6:2022, Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full — Part 6: Wedge meters</std>~~

ISO 4006, Measurement of fluid flow in closed conduits — Vocabulary and symbols

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 4006 apply.

### 4 How the structure of this guide relates to ISO 5167:2022 ~~(all parts) series~~

Clause 5 of this ~~Technical Report~~ document sets out the guidance specific to each of the ~~four~~ six parts of ISO 5167:2022:

- 5.1 covers part 1;
- 5.2 covers part 2;
- 5.3 covers part 3;
- 5.4 covers part 4;
- 5.5 covers part 5;
- 5.6 covers part 6.

Subsequent subclause numbering relates to the clauses in each of the parts. Hence, 5.1.1 covers Clause 1 in ~~part ISO 5167-1:2022~~; ~~5.4.3.1.1~~ covers ~~Subclause 3.1.1~~ in ~~part ISO 5167-4:2022~~.

Guidance applicable to all ~~four~~ six parts is given in Clause 6.

### 5 Guidance on the use of ISO 5167:2022 ~~(all parts) series~~

#### 5.1 Guidance specific to the use of ISO 5167-1:2022

##### 5.1.1 Scope

No comments on this clause.

##### 5.1.2 Normative references

No comments on this clause.

##### 5.1.3 Terms and definitions

No comments on this clause.

##### 5.1.4 Symbols and subscripts

No comments on this clause.

**Commented [eXtyle1]:** Not found, but similar references exist

ISO 5167 (all parts), — Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full

**Formatted:** Pattern: Clear

**Formatted:** Pattern: Clear

**Formatted:** Pattern: Clear

**Commented [eXtyle3]:** No section matches the in-text citation "5.4.3.1.1". Please supply the missing section or delete the citation.

**Formatted:** std\_docPartNumber

**Formatted:** cite\_sec

**Formatted:** std\_section

**Formatted:** std\_docPartNumber

**Commented [eXtyle5]:** Not found, but similar references exist

ISO 5167 (all parts), — Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full



### 5.1.5 Principle of the method of measurement and computation

#### 5.1.5.1 Principle of the method of measurement

No comments on this subclause.

#### 5.1.5.2 Method of determination of the diameter ratio of the standard primary device

See Annex A of this Technical Report.

#### 5.1.5.3 Computation of flowrate

The equations/formulae to be used to determine the flowrate of a measuring system are given in ISO 5167-1:2022, Clause 5. Some results of these calculations will be fixed with installation dimensions and will only need to be computed once. Other calculations will need to be repeated for every flow measurement point. Annex A gives worked examples of the iterative computations shown in ISO 5167-1:2022, Annex A.

#### 5.1.5.4 Determination of density, pressure and temperature

##### 5.1.5.4.1 General

No comments on this subclause.

##### 5.1.5.4.2 Density

For details on density measurement, see 6.4.

For details on density computation, see Annex B of this Technical Report.

##### 5.1.5.4.3 Static pressure

No comments on this subclause.

##### 5.1.5.4.4 Temperature

The computation of temperature decrease resulting from expansion of the fluid through the primary device requires knowledge of the Joule-Thomson coefficient. The coefficient is a function of temperature, pressure and gas composition. The calculation can be carried out using an equation of state (see, in Annex B, the “detailed method” using molar composition analysis) or by the use of an approximation valid for natural gas mixtures that are not too rich, and when  $p$  and  $T$  are in the range given below. In the last case, the coefficient is a function of  $p$  and  $T$  alone.

Provided that, in the molar composition of the natural gas, methane is greater than 80 %, the temperature is in the range 0 °C to 100 °C and the absolute static pressure is in the range 100 kPa to 20 MPa (1 bar to 200 bar)

$$\mu_{JT} = 0,35 - 0,001\,42t + (0,231 - 0,002\,94t + 0,000\,013\,6t^2) (0,998 + 0,000\,41p - 0,000\,111\,5p^2 + 0,000\,000\,3p^3) \quad (1)$$

where

$\mu_{JT}$  is the Joule-Thomson coefficient, in kelvin per bar (K/bar);

$t$  is the temperature of the fluid, in degrees Celsius (°C);

$p$  is the absolute static pressure of the fluid, in bar.

## ISO/DTR 9464:2023(E)

The uncertainty was determined from the differences between this equation and the Joule-Thomson coefficient of 14 common natural gases and is given by

$$U = 0,066 \left( 1 - \frac{t}{200} \right) \quad \text{for } p \leq 70 \text{ bar (7 MPa)} \quad (2)$$

and

$$U = 0,066 \left( 1 - \frac{t}{200} \right) \left[ 1 - \frac{(290-t)}{4} \left( \frac{1}{70} - \frac{1}{p} \right) \right] \quad \text{for } p > 70 \text{ bar (7 MPa)} \quad (3)$$

where  $U$  is the expanded uncertainty in the Joule-Thomson coefficient (K/bar) at  $k = 2$  (approximately 95 % confidence level).

NOTE If an orifice plate with  $\beta = 0,6$  has a differential pressure  $\Delta p = 0,5$  bar, the uncertainty in the Joule-Thomson coefficient corresponds to an expanded uncertainty in flowrate in the range from 0,001 % to 0,009 % at  $k = 2$  (approximately 95 % confidence level), depending on the temperature, the pressure and the gas composition.

### 5.1.5.5 Differential pressure flow measurement system

No comments on this subclause.

### 5.1.5.6 Differential pressure flow measurement system design considerations

5.1.5.6.1 No comments on this subclause.

5.1.5.6.2 No comments on this subclause.

5.1.5.6.3 When comparing the permanent pressure loss with alternative differential pressure meter designs, it is important to compare meter designs that are sized to provide a similar range of differential pressure, rather than to compare different meter designs with the same value of  $\beta$ .

5.1.5.6.4 No comments on this subclause.

5.1.5.6.5 No comments on this subclause.

### 5.1.6 General requirements for the measurements

#### 5.1.6.1 Primary device

5.1.6.1.1 No comments on this subclause.

5.1.6.1.2 No comments on this subclause.

5.1.6.1.3 Table 1, although not exhaustive, lists materials most commonly used for the manufacture of primary devices.

Table 1 — Steels commonly used for the manufacture of primary devices

	ASTM/AISI	BS 970	AFNOR	DIN
Stainless steels	304	304-S15	Z6CN18-09	1.4301
	316	316-S16	Z6CND17-11	1.4401

Formatted: Default Paragraph Font, Font: Not Bold

Formatted: Default Paragraph Font, Font: Not Bold

High elastic limit stainless steel	420	420-S37	Z30C13	
------------------------------------	-----	---------	--------	--

Table 2 gives the mean linear expansion coefficient, elasticity moduli and yield stresses for the materials of Table 1 according to their ASTM/AISI designation.

**Table 2 — Typical characteristics of commonly used steels**

ASTM/AISI designation	Mean linear expansion coefficient between 0 °C and 100 °C K <sup>-1</sup>	Elasticity modulus Pa	Yield stress Pa
304	$17 \times 10^{-6}$	$193 \times 10^9$	$215 \times 10^6$
316	$16 \times 10^{-6}$	$193 \times 10^9$	$230 \times 10^6$
420	$10 \times 10^{-6}$	$200 \times 10^9$	$494 \times 10^6$

The values given in Table 2 vary with both temperature and the treatment process of the steel. For precise calculations, it is recommended that the data are obtained from the manufacturer.

When the primary device under operating conditions is at a different temperature from the one at which the diameter “*d*” was determined (this temperature is referred to as the reference or calibration temperature), it is necessary to calculate the expansion or contraction of the primary device. The corrected diameter “*d*” to be used in the computation of diameter ratio and flowrate is calculated using Equation (4), assuming there is no restraint due to the mounting:

$$d = d_0 [1 + \lambda_d (T - T_0)] \quad (4)$$

where

*d* is the primary device diameter in flowing conditions;

*d*<sub>0</sub> is the primary device diameter at reference temperature;

$\lambda_d$  is the mean linear expansion coefficient of the primary device material;

*T* is the primary device temperature in flowing conditions;

*T*<sub>0</sub> is the reference or calibration temperature.

Where automatic temperature correction is not required in the flow computer, the uncertainty for “*d*” included in the overall uncertainty calculations is increased for the change in “*d*” due to temperature variation (see ISO 5167-1:2022, 8.3.2.4). An initial calculation might show that this additional uncertainty is small enough to be considered negligible.

#### 5.1.6.2 Nature of the fluid

No comments on this subclause.

#### 5.1.6.3 Flow conditions

5.1.6.3.1 No comments on this subclause.

5.1.6.3.2 No comments on this subclause.

5.1.6.3.3 No comments on this subclause.

**Formatted:** Adjust space between Latin and Asian text, Adjust space between Asian text and numbers, Tab stops: Not at 19.85 pt + 39.7 pt + 59.55 pt + 79.4 pt + 99.25 pt + 119.05 pt + 138.9 pt + 158.75 pt + 178.6 pt + 198.45 pt

**Field Code Changed**

**Formatted:** Subscript, Not Raised by / Lowered by

**Formatted:** Subscript, Not Raised by / Lowered by

**Formatted:** Subscript, Not Raised by / Lowered by

## ISO/DTR 9464:2023(E)

### 5.1.7 Installation requirements

#### 5.1.7.1 General

The following list of inspection equipment is not exhaustive, but provides a basis for inspection control:

- calipers (thickness, diameters);
- internal micrometer (diameters);
- micrometer (thickness);
- gauge block, feeler gauge (relative position, absolute standard for checking micrometers);
- protractor (angles);
- profile measuring apparatus (edge);
- straight edge rule (flatness);
- three point bore gauge (internal diameter).

It is necessary only to use instruments that can be calibrated to primary standards if optimum accuracy is required.

5.1.7.1.1 No comments on this subclause.

5.1.7.1.2 No comments on this subclause.

5.1.7.1.3 No comments on this subclause.


5.1.7.1.4 No comments on this subclause.

5.1.7.1.5 No comments on this subclause.

5.1.7.1.6 The requirements in this subclause of ISO 5167-1, where drain or vent holes are located near to the primary device, are illustrated in Figure 1. This figure illustrates the importance of placing the drain or vent hole in the annular chamber where one is used. The location of a drain or vent hole relative to a pressure tapping is of greater importance where there is no annular chamber and the drain or vent hole enters the pipe itself.

The flowing fluid might cause deposition, corrosion or erosion of the inner wall of the pipe. The installation might therefore not conform to the requirements of ISO 5167-1. Internal inspection of the pipe is carried out at intervals appropriate to the conditions of application.

9464\_ed3fig1.EPS

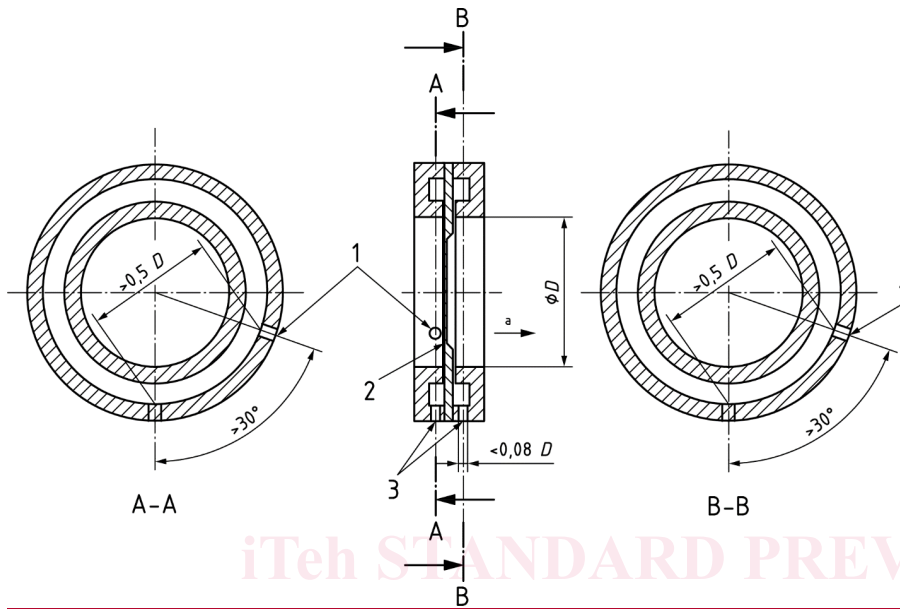

## Key

- 1 pressure tapping
- 2 orifice plate
- 3 drain holes and/or vent holes
- a Flow direction.

iTech STANDARD PREVIEW  
(standards.iteh.ai)  
ISO/DTR 9464  
<https://standards.iteh.ai/catalog/standards/sist/80993c42-ee5-41d1-b8c5-dtr-9464>  
**Figure 1 — Location of drain holes and/or vent holes**

**5.1.7.1.7** This subclause is intended to ensure a reliable measurement of temperature. The flowing temperature is an important parameter since it is used in calculating the density of the flowing fluid and is used to calculate  $d$  and  $D$ . Furthermore, it is used to calculate critical process parameters under flowing conditions.

#### 5.1.7.2 Minimum upstream and downstream straight lengths

**5.1.7.2.1** No comments on this subclause.

**5.1.7.2.2** When designing a metering pipe installation, it is recommended that the required minimum straight lengths are determined by the maximum diameter ratio that is expected in the life of the installation.

For diameter ratios not actually shown in ISO 5167-2:2022, Table 3, ISO 5167-3:2022, Table 3 or ISO 5167-4:2022, Table 1 but which are inside the limits of the standard, it is reasonable practice to interpolate linearly between the values obtained at the nearest two diameter ratios.

**ISO/DTR 9464:2023(E)**

If an orifice meter is designed to measure the flowrate in either direction, the minimum requirements for upstream and downstream straight lengths as specified in ISO 5167-2:2022, 6.2 and Table 3 are applicable on both sides of the orifice plate.

**5.1.7.3 General requirement for flow conditions at the primary device**

No comments on this subclause.

**5.1.7.4 Flow conditioners**

Although swirl is generally not detectable in visual inspection of the pipe, swirl and asymmetry are sometimes visible in the coating, if present, on an orifice plate. A typical herring bone or chevron pattern that is seen on a plate that has been in service for some time might indicate that the flow at the orifice plate is swirling or asymmetrical. Swirl has a greater effect on measurement than any other fluid dynamic mechanism and, although straight lengths of pipe will eliminate swirl, decay occurs very slowly and the swirl persists over considerable distances.

Flow conditioners are strongly recommended where the upstream fittings or arrangement of fittings are not defined in the tables, e.g. a metering system header. They can also be useful to reduce the required upstream length. However, the additional permanent pressure loss induced by a flow conditioner is also a consideration.

ISO 5167-1:2022 describes compliance testing for flow conditioners.

**5.1.8 Uncertainty on the measurement of flowrate**

ISO/IEC Guide 98-3 *Uncertainty of measurement — Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)* (Reference [4])<sup>[12]</sup> and ISO 5168 (Reference [1])<sup>[9]</sup> are taken into account when performing uncertainty analyses.

Careful study of any manufacturer’s specification of uncertainty helps to ensure that the metering system uncertainty is known at the measured value concerned. Some points to note include the following:

- a) uncertainties are often expressed as a percentage of full scale or range;
- b) uncertainties are often defined at specified reference conditions. Additional uncertainties might arise when operating conditions differ from reference conditions.

**5.2 Guidance specific to the use of ISO 5167-2:2022**

**5.2.1 Scope**

This part of ISO 5167-2:2022 is concerned solely with orifice plates and their geometry and installation. It is necessary to read ISO 5167-2 in conjunction with ISO 5167-1.


Orifice plate meters with three arrangements of tapings are described and specified: flange tapings; corner tapings; and *D* and *D*/2 tapings.

**5.2.2 Normative references**

No comments on this clause.

**5.2.3 Terms, definitions and symbols**

No comments on this clause.

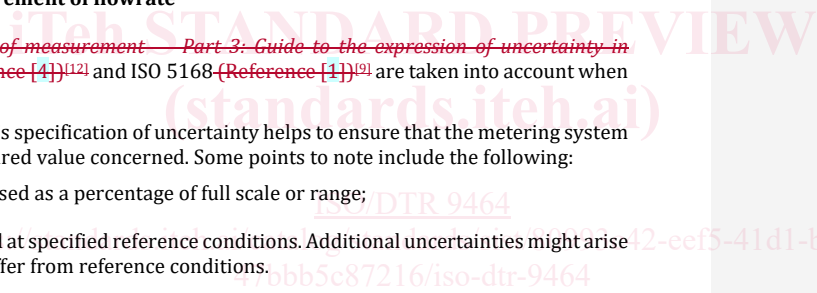

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

Formatted: Pattern: Clear

#### 5.2.4 Principles of the method of measurement and computation

The density and viscosity of the fluid can be measured (see 6.4) or calculated (see Annex B) from the gas composition. A number of computer programs are available for carrying out the calculation of density and viscosity. In the case of a compressible fluid, the isentropic exponent at working conditions is necessary for the flow calculation and this can be calculated from gas composition.

#### 5.2.5 Orifice plates

##### 5.2.5.1 Description

###### 5.2.5.1.1 General

No comments on this subclause.

###### 5.2.5.1.2 General shape

5.2.5.1.2.1 No comments on this subclause.

5.2.5.1.2.2 No comments on this subclause.

5.2.5.1.2.3 Referring to Annex C, three rules need to be taken into consideration in designing an orifice plate to avoid excessive deformation:

- Firstly, that the mounting arrangements are such that no forces are imposed on the orifice plate which would cause the limit of 0,5 % slope given in ISO 5167-2:2022, 5.1.3.1 to be exceeded under the condition of no differential pressure.
- Secondly, that the thickness of the plate,  $E$ , is such that, taking account of the modulus of elasticity of the plate material, the differential pressure for the maximum design flowrate does not cause a 1 % slope to be exceeded. When the flowrate is reduced to zero, the plate will return to the original maximum 0,5 % slope.
- Thirdly, that, if it is possible for differential pressures in excess of those for maximum design flowrate to be applied, plastic buckling (i.e. permanent deformation) does not occur.

For the first point, great care is needed in both the design and the manufacture of the mounting arrangements. Single or double chamber mounting devices are satisfactory. When mounting orifice plates correctly between standard flanges, the flanges are at  $90^\circ \pm 1^\circ$  to the pipe axis. The pipe sections on both sides of the orifice plate are adequately supported to ensure that no undue strain is placed on the orifice plate.

For the second point, it is clear that elastic deformation of an orifice plate introduces an error in the flow measurement results. As long as the deformation does not exceed the 1 % slope required by ISO 5167-2:2022, 5.1.2.3, no additional uncertainty will result. Theoretical and experimental research (see Reference [1321]) indicates that the maximum change in discharge coefficient for a 1 % slope is 0,2 %. Therefore, orifice plates that conform to the 0,5 % slope specified in ISO 5167-2:2022, 5.1.3.1 can deform an additional 0,5 % slope (i.e. 0,1 % change in discharge coefficient) while still conforming to the requirements of this subclause. Table 3 tabulates the plate thickness to plate support diameter ratio ( $E/D$ ) for various values of  $\beta$  and differential pressures, valid for an orifice plate manufactured from ASTM/AISI stainless steel 304 or 316, and simply supported at its rim.

**Table 3 — Minimum  $E/D$  ratios for orifice plates manufactured in ASTM/AISI 304 or ASTM/AISI 316 stainless steel**