

ISO-/DTR 14644-21:2023(E)

ISO/TC-209 WG-15

Secretariat: ANSI/AESF

Date: 2023-05-30

ISO/DTR 14644-21:2023 — Cleanrooms and associated controlled environments —
Airborne particle sampling techniques

~~DTR stage~~

Warning for WDs and CDs

This document is not an ISO International Standard. It is distributed for review and comment. It is subject to change without notice and may not be referred to as an International Standard.

Recipients of this draft are invited to submit, with their comments, notification of any relevant patent rights of which they are aware and to provide supporting documentation.

[ISO/DTR 14644-21](https://standards.iteh.ai/catalog/standards/sist/9c6a38ef-195d-4b06-a086-536c0c6b1d59/iso-dtr-14644-21)

<https://standards.iteh.ai/catalog/standards/sist/9c6a38ef-195d-4b06-a086-536c0c6b1d59/iso-dtr-14644-21>

ISO/DTR 14644-21:2023(E)

| © ISO 2022

iTeh STANDARD PREVIEW (standards.iteh.ai)

ISO/DTR 14644-21

<https://standards.iteh.ai/catalog/standards/sist/9c6a38ef-195d-4b06-a086-536c0c6b1d59/iso-dtr-14644-21>

ISO/DTR 14644-21:2023(E)

© ISO 2023

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office Copyright Office

CP 401 • Ch. de Blandonnet 8

CH-1214 Vernier, Geneva

Phone: +41 22 749 01 11

Email: copyright@iso.org

Email: copyright@iso.org

Website: www.iso.org

Published in Switzerland.

iTeh STANDARD PREVIEW
(standards.iteh.ai)

ISO/DTR 14644-21

<https://standards.iteh.ai/catalog/standards/sist/9c6a38ef-195d-4b06-a086-536c0c6b1d59/iso-dtr-14644-21>

Contents

Foreword.....	4
Introduction	5
1 Scope.....	6
2 Normative documents.....	6
3 Terms and definitions.....	6
4 Determination of airborne particle concentration	7
4.1 General.....	7
4.2 Classification	8
4.3 Monitoring	9
4.4 Other LSAPC Applications.....	10
5 Sampling Airborne Particles – Things to Consider	10
5.1 General.....	10
5.2 Instrument Selection	10
5.2.1 Considered Particle Size Selection	11
5.2.2 Required sample volume and sample flow rate	12
5.3 State of Occupancy	12
5.4 Sample Locations – points to consider.....	12
5.4.1 Sampling Locations for Classification	12
5.4.2 Sample Locations for Monitoring	14
5.5 Instrument Measurement Issues.....	15
5.5.1 Sampling Errors	15
5.5.2 Sample Measurement Errors.....	17
5.5.3 Sample tubing issues	19
5.6 Decision Tree	21
5.7 Examples of use of the Decision Tree.....	23
5.7.1 Example 1.....	23
5.7.2 Example 2.....	25
5.7.3 Example 3.....	26
6 Verifying a System.....	28
Bibliography.....	29

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part-1. In particular, the different approval criteria needed for the different types of ISO ~~documents~~document should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

~~Attention is drawn~~ISO draws attention to the possibility that ~~some of the elements~~implementation of this document may ~~be involve~~ the ~~subject~~use of (a) patent(s). ISO takes no position concerning the evidence, validity or applicability of any claimed patent rights in respect thereof. As of the date of publication of this document, ISO had not received notice of (a) patent(s) which may be required to implement this document. However, implementers are cautioned that this may not represent the latest information, which may be obtained from the patent database available at www.iso.org/patents. ISO shall not be held responsible for identifying any or all such patent rights. ~~Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).~~

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This ~~Technical Report (ISO TR 14644-21)~~document was prepared by ISO/TC 209 (Cleanrooms and associated controlled environments)

A list of all parts in the ISO 14644 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

This ~~Technical Report (TR)~~document provides clarification on the application of sound airborne particle sampling techniques in ~~accordance with~~support of ISO 14644-1:2015 for classification of cleanrooms and clean zones, and ISO 14644-2:2015 for airborne particle monitoring, to provide evidence of cleanroom performance related to air cleanliness by particle concentration. It provides information on how to gather appropriate, accurate and repeatable data, and how to interpret this information for the purpose of improving process protection. ~~This also includes~~ information on the choice of measurement methods and apparatus configuration, calibration, repeatability/reproducibility and the uncertainty associated with measurement. In short, what can be reasonably attained with the current technology.

This ~~TR~~document addresses potential misinterpretation of the use of ~~clause~~ISO14644-1:2015, C.4.1.2 in informative ~~annex-Annex C of ISO14644-1~~, which suggests the use of limited tubing length for sampling macroparticles. The phrase in question has been applied beyond the context intended in ~~the Standard~~ISO14644-1, to other applications. This ~~TR~~document also provides extra clarity on the use of the M Descriptor in ~~ISO14644-1:2015, Annex-C~~, specifically in relation to consideration of ~~$\geq 5,0 \mu\text{m}$~~ $\geq 5,0 \mu\text{m}$ alongside ISO Class 5 (EU-PIC/S GMP Grade A and B at rest).

It provides information on the potential uncertainty associated with sampling particles $\geq 5,0 \mu\text{m}$ and macro-particles, and measures that can be taken to reduce that uncertainty.

It addresses the importance of understanding that:

~~For~~ for classification, the quality of the sample is the most important factor;

~~For~~ for monitoring, the quality of the data is the most important factor;

~~Direct~~ direct sampling without tubing is preferred. However, sample tubing is sometimes necessary to get a representative sample at a significant or critical location;

~~To~~ to reduce sampling loss in tubing, this tubing is as short and straight as possible;

~~A~~ a sampling system is evaluated to assess the impact of any compromises in its set up. |

An evaluation of legacy systems can deem them suitable for continued use even if the installation is assessed as less than optimal

The scientific basis for airborne particle counting, and the performance characteristics of airborne particle counters, particularly LSAPC, is amply documented in established technical publications (see Bibliography)

Cleanrooms and associated controlled environments — Part 21: Airborne particle sampling techniques

1 Scope

This ~~TR~~document discusses the physical limitations of probe and particle counter placement, and any tubing that connects the two, particularly in providing representative samples where particles 5 micrometres and greater are of interest.

The document further identifies the key factors of sampling performance when classifying and monitoring, and good practice to determine and maintain an acceptable compromise between attainable accuracy in counting and feasibility of counting in real-life situations.

This ~~TR~~document includes a decision tree, used to identify key considerations when sampling airborne particles, and whether the system requires further assessment. There are also examples provided to illustrate typical application challenges and show how the decision tree can be used.

It is assumed that this ~~TR~~document is read in conjunction with ISO 14644-~~parts~~-1 and ISO 14644-2. This ~~TR~~document is not a manual, but an explanatory document. It does not describe measurement methods, which is handled in ISO 14644-~~parts~~-1 and ISO 14644-2, but provides information to help make effective choices of sampling configuration, when evaluating a new or existing system.

2 Normative documents

~~This ISO/TR provides guidance on the use of the following normative documents. For dated references, subsequent amendments to, or revisions of, any of these publications do not apply. For undated references, the latest edition of the normative document referred to applies. Members of ISO and IEC maintain registers of currently valid International Standards.~~

There are no normative references in this document.

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org>

3.1

classification

method of assessing level of cleanliness against a specification for a cleanroom or clean zone

Formatted: Font: 11 pt

Note 1 to entry: Levels should be expressed in terms of an ISO Class, which represents maximum allowable concentrations of particles in a unit volume of air.

[SOURCE: ISO 14644-1:2015, 3.1.4]

3.2 monitoring

observations made by measurement in accordance with a defined method and plan to provide evidence of the performance of an installation

Note 1 to entry: Monitoring may be continuous, sequential or periodic; and if periodic, the frequency shall be specified.

Note 2 to entry: This information may be used to detect trends in operational state and to provide process support.

[SOURCE: ISO 14644-2:2015, 3.2]

3.3 particle size

diameter of a sphere that produces a response, by a given particle-sizing instrument, that is equivalent to the response produced by the particle being measured

Note 1 to entry: For discrete-particle light-scattering instruments, the equivalent optical diameter is used.

[SOURCE: ISO 14644-1:2015, 3.2.2]

3.4 macroparticle

particle with an equivalent diameter greater than 5-µm

[SOURCE: ISO 14644-1:2015, 3.2.5]

3.5 M descriptor

designation for measured or specified concentration of macroparticles per cubic metre of air, expressed in terms of the equivalent diameter that is characteristic of the measurement method used

Note 1 to entry: The M descriptor can be regarded as an upper limit for the averages at sampling locations. M

_descriptors cannot be used to define air cleanliness classes by particle concentration, but they may be quoted independently or in conjunction with air cleanliness classes by particle concentration.

[SOURCE: ISO 14644-1:2015, 3.2.6]

Formatted: Font: 11 pt

Formatted: Space After: 12 pt, Line spacing: Exactly 11 pt

2 © ISO 2023 – All rights reserved

2 © ISO 2023 – All rights reserved

4 Determination of airborne particle concentration

4.1 –General

Airborne particle concentration is the primary attribute and essential parameter that determines and denotes the air cleanliness level of a cleanroom or clean zone.

In classification, ISO 14644-1 states that “The use of light scattering (discrete) airborne particle counters (LSAPC) is the basis for determination of the concentration of airborne particles, equal to and greater than the specified sizes, at designated sampling locations.


This part of ISO 14644-1 does not provide for classification of particle populations that are outside the specified lower threshold particle-size range, 0,1-µm to 5-µm. An M descriptor (see Annex-C) may be used to quantify populations of macroparticles (particles larger than 5-µm)”.

In monitoring, an LSAPC is also used for airborne particle counting, often supported by other methods, as indicated in ISO 14644-2.

For both classification and monitoring, the choice of the counter takes account of the effective particle size range and sampling flowrate with regard to sample size.

For monitoring, the effectiveness of the sampling system is determined by the appropriate choice of sampling location and the ability of the system to capture particles and deliver them to the counting mechanism.

A key driver in quality management is continuous improvement. When we apply the dynamic cycle tool Plan-Do-Check-Act (PDCA) to cleanroom contamination control, key information is used from classification and monitoring activities to establish and demonstrate that control. Changes and improvements will lead to re-evaluation and a repeat of this cycle. Figure_1 below illustrates the importance of classification and monitoring and how these influence the process of continual improvement.

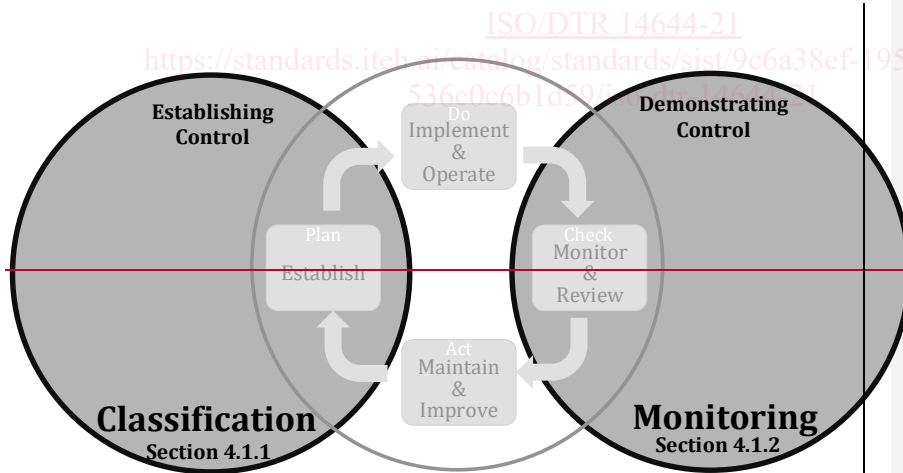

Formatted: Font: 11 pt
Formatted: Space After: 12 pt, Line spacing: Exactly 11 pt

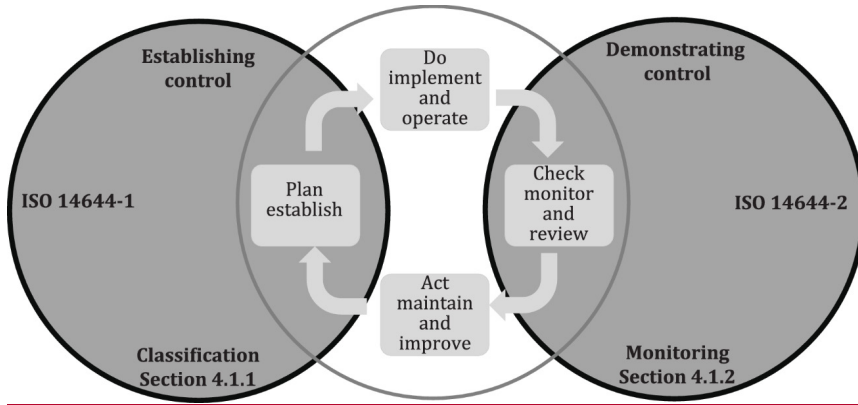


Figure 1 – Strategy for Contamination Control

All particle counting systems have the potential to delay or prevent a particle from reaching the counting mechanism of the LSAPC. The likelihood of this increases with the particle's size and the length and complexity of its pathway through the system. Good practice is applied to minimise particle loss ~~(or and potential gain through shedding and false counts/gain)~~. The following sections explain the relevant aspects of the determination of airborne particle concentration that is performed in classification and monitoring. Guidance will be given in chapter 5 on the application of particle counting technologies and associated sampling methods.

4.2 –Classification

In classification, the cleanliness of the cleanroom is specified for a state of occupancy and considered particle size(s). The sizes available for classification are defined in Table_1 of ISO 14644-1:2015, and all sizes considered are measured simultaneously, with the same LSAPC instrument. Sampling locations and minimum sample volumes are selected using the procedure described in ISO 14644-1. Satisfactory airborne particle concentration results obtained by sampling at these locations provide confidence that the volume measured will comply with the specified class.

The reference method for classification supposes a degree of reproducibility to establish control for a specified state of occupation, both initially and when classification is reconfirmed. As such, the quality of the sample taken and precision of the values recorded is paramount.

The measurement of airborne nanoscale particles, ~~<0.1µm, 1 µm~~, uses another type of instrument, not included in this ~~TRdocument~~. Values obtained at the nanoscale are not appropriate for classification. This application is considered in ISO 14644-12.

Table_1 of ISO 14644-1:–2015 provides the range of particle sizes and particle concentrations deemed statistically appropriate for classification.

NOTE: ~~In~~ ISO 14644-1, Table_E.1 shows application of the same threshold particle sizes for decimal classes, and ISO 14644-1, Formula_E.1 enables calculation of the maximum particle concentration for intermediate particle sizes within the normative range.

4 © ISO 2023 – All rights reserved

4 © ISO 2023 – All rights reserved

Note f) to Table 1 of ISO 14644-1:2015 indicates a special case for recording larger particles when classifying at ISO 5. It provides an example where particles $\geq 5 \mu\text{m}$ are sampled with a specified limit of 29 particles per m^3 as a complement to classification at ISO 5 measured on sizes that are included in ISO 14644-1:2015, Table 1 as appropriate for that class. This complement is expressed via the M Descriptor, in this case as "ISO M (29; $\geq 5 \mu\text{m}$); LSAPC". for ISO 5. In this respect, Note f) below Table 1 of ISO 14644-1:2015 refers on to clause ISO 14644-1:2015, C.7 of informative Annex C of the standard. For some applications, it can be necessary to also sample other sizes outside those for which Table 1 of ISO 14644-1:2015 defines concentrations. Clause ISO 14644-1:2015, C.7 in informative annex C of the standard Annex C provides an example of adaptation of the M descriptor to accommodate consideration of $\geq 5 \mu\text{m}$ particle size for ISO Class 5 at this particle size threshold, where ISO 14644-1:2015, Table 1 does not specify a concentration limit.

Annex C of ISO 14644-1:2015 is concerned with the broader techniques of measurement of macroparticles (particle size thresholds not in ISO 14644-1:2015, Table 1), by a variety of appropriate methods and instrumentation, including the LSAPC, and expression of the result. This subject is not considered within the scope of this Technical Report document. When measuring and recording particles $> 5 \mu\text{m}$ (macroparticles) alongside those measured within the ISO 14644-1:2015, Table 1 range, their value is expressed as an M descriptor, in support of classification.

4.3 –Monitoring

Monitoring is explained and illustrated in ISO 14644-2:2015. The activity involves recording and analysing data on a variety of parameters to support demonstration of control.

The trending of data obtained from monitoring with LSAPC is used to understand the variation in the number of particles over time and its relationship with the specified and maintained cleanliness of the cleanroom or clean zone. Data obtained and analysed serves to indicate that air quality is maintained at a satisfactory level at locations considered significant or critical for the process, at the appropriate occasions. This data can be analysed along with other monitoring parameters to provide a holistic approach to demonstrating control.

Monitoring is applied to demonstrate that the air cleanliness at a defined location complies with the required level at a defined point in time, during operation, and often during periods at rest. Particle sizes used for monitoring can be different from those required for classification. This is clearly shown in EU & PIC/S GMP Annex 1 (2022) where monitoring is subject to limits for particle sizes ($> 5 \mu\text{m}$) not identified as reliable for the purpose of classification at ISO 5. Results are often expressed per unit of time, rather than accumulated to a unit volume. Other indirect indicators may also inform on the satisfactory operation of the installation or equipment.

In ISO 14644-2: guidance is provided on where, when and how to monitor the airborne particle concentration, and how to complement this with other indicators of cleanroom or process zone performance.

In monitoring, the reproducibility of sampling efficiency, and the ability to detect variations over time, are more important than absolute precision in the data obtained.

Analysis of variations over time can help to understand the process, and provide trending data to assist the management of critical parameters in order to maintain control as required.

Monitoring performed using a mobile or fixed LSAPC can be periodic or continuous. In monitoring, minor particle loss in the sampling system is typically accepted since this will not affect the trending of the local air cleanliness unless the alert or action level is very low.

© ISO 2023 – All rights reserved

© ISO 2023 – All rights reserved

Formatted: Font: 11 pt

Formatted: Space After: 12 pt, Line spacing: Exactly 11 pt