



Designation: C336 – 71 (Reapproved 2015)

Standard Test Method for Annealing Point and Strain Point of Glass by Fiber Elongation¹

This standard is issued under the fixed designation C336; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This standard has been approved for use by agencies of the U.S. Department of Defense.

1. Scope

1.1 This test method covers the determination of the annealing point and the strain point of a glass by measuring the viscous elongation rate of a fiber of the glass under prescribed condition.

1.2 The annealing and strain points shall be obtained by following the specified procedure after calibration of the apparatus using fibers of standard glasses having known annealing and strain points, such as those specified and certified by the National Institute of Standards and Technology (NIST)² (see [Appendix X1](#)).

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*³

[C338 Test Method for Softening Point of Glass](#)

[C598 Test Method for Annealing Point and Strain Point of Glass by Beam Bending](#)

¹ This test method is under the jurisdiction of ASTM Committee C14 on Glass and Glass Products and is the direct responsibility of Subcommittee C14.04 on Physical and Mechanical Properties.

Current edition approved May 1, 2015. Published May 2015. Originally approved in 1954. Last previous edition approved in 2010 as C336 – 71 (2010). DOI: 10.1520/C0336-71R15.

² Available from National Institute of Standards and Technology (NIST), 100 Bureau Dr., Stop 1070, Gaithersburg, MD 20899-1070, <http://www.nist.gov>. Publication 260.

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

3. Definitions

3.1 *annealing point*—that temperature at which internal stresses in a glass are substantially relieved in a matter of minutes.^{4,5,6} During a test in accordance with the requirements of this method, the viscous elongation rate is measured by a suitable extensometer while the specimen fiber is cooling at a rate of $4 \pm 1^\circ\text{C}/\text{min}$. The elongation rate at the annealing point is approximately 0.14 mm/min for a fiber of 0.65 mm diameter.⁶

3.2 *annealing range*—the range of glass temperature in which stresses in glass articles can be relieved at a commercially desirable rate. For purposes of comparing glasses, the annealing range is assumed to correspond with the temperatures between the annealing point (AP) and the strain point (StP).

3.3 *strain point*—that temperature at which the internal stresses in a glass are substantially relieved in a matter of hours. The strain point is determined by extrapolation of the annealing point data and is the temperature at which the viscous elongation rate is 0.0316 times that observed at the annealing point.

4. Significance and Use

4.1 This test method provides data useful for (1) estimating stress release, (2) the development of proper annealing schedules, and (3) estimating setting points for seals.

⁴ Littleton, J. T., and Roberts, E. H., "A Method for Determining the Annealing Temperature of Glass," *Journal of the Optical Society of America*, Vol 4, 1920, p. 224.

⁵ Lillie, H. R., "Viscosity of Glass Between the Strain Point and Melting Temperature," *Journal of American Ceramic Society*, Vol 14, 1931, p. 502; "Re-Evaluation of Glass Viscosities at Annealing and Strain Points," *Journal of American Ceramic Society*, Vol 37, 1954, p. 111.

⁶ McGraw, D. A. and Babcock, C. L., "Effect of Viscosity and Stress Level on Rate of Stress Release in Soda-Lime, Potash-Barium and Borosilicate Glasses," *Journal of the American Ceramic Society*, Vol 42, 1959, p. 330.

Accordingly, its usage is widespread throughout manufacturing, research, and development. It can be utilized for specification acceptance.

5. Apparatus

5.1 *Furnace*—The furnace shall be 368 mm (14½-in.) long and approximately 114 mm (4½ in.) in diameter and shall contain a copper core 305 mm (12 in.) long and 29 mm (1⅛ in.) in outside diameter, with inside diameter of 5.6 mm (⅞ in.). It shall be constructed substantially as shown in Fig. 1.


5.1.1 Such a furnace will cool naturally at approximately 4°C (7°F)/min at 500°C (932°F) and at a rate exceeding 3°C (5.5°F)/min at 400°C (752°F).

5.2 *Temperature Measuring and Indicating Instruments*—For the measurement of temperature there shall be provided a thermocouple, preferably platinum-platinum rhodium, inserted in the upper side hole of the copper core, as indicated in Fig. 1, so that its junction is located midway in the length of the core. The thermocouple wire shall not be allowed to directly

contact the copper; this can be ensured by placing a 6 mm (¼-in.) length of ceramic tube in the bottom of the hole ahead of the couple. The cold junction of the thermocouple shall be maintained in an ice bath during tests.

5.2.1 The temperature-indicating instrument, preferably a potentiometer, shall be of such quality and sensitivity as to permit reading the thermocouple emf to an amount corresponding to 0.1°C (0.2°F), equivalent to about 1 μV for a platinum couple or to about 4 μV for a base-metal couple.

5.2.2 Provision shall be made for reading temperatures accurately at predetermined moments. One means of accomplishing this is to maintain the potentiometer setting at an electromotive force corresponding to a known temperature, near the annealing point and inferring the temperature from the deflection of a sensitive galvanometer, previously calibrated for the purpose. It is convenient to adjust the galvanometer shunt to a sensitivity of about 3°C (5.5°F)/cm of deflection and to somewhat less than critical damping. This technique for reading temperature changes is one of the preferred methods; in the following sections it will be assumed that this technique

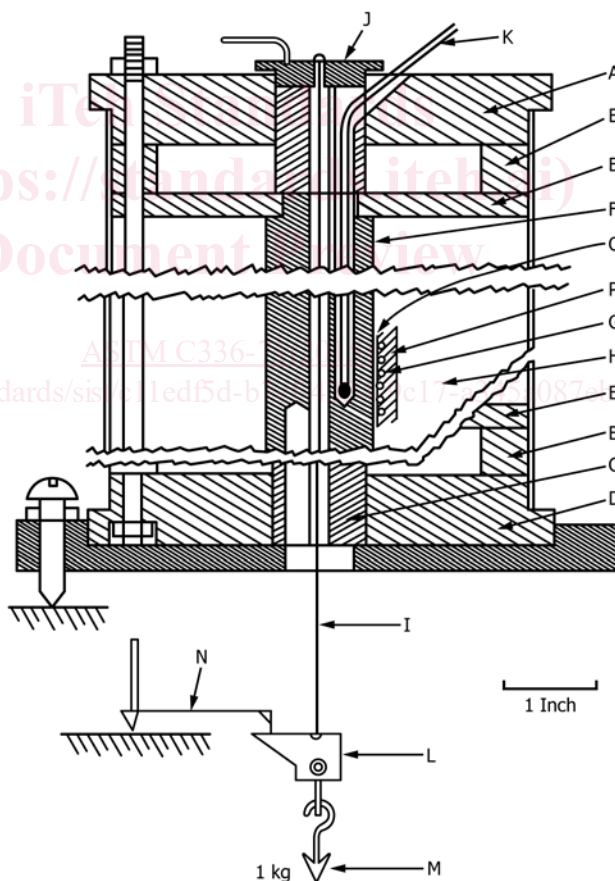

- A, B, C, D—Made of asbestos-cement (Transite or equivalent)
- E—Webbed asbestos-cement (Transite or equivalent) disk
- F—Copper core 1⅛ in. (29 mm) outside diameter by 12 in. (305 mm) total length (Note)
- G—91 turns No. 22 Nichrome V wire (or equivalent)
- H—Diatomaceous earth
- I—Sample fiber
- J—Stainless steel support disk

- K—Thermocouple
- L—Lever platform
- M—Load
- N—Optical lever
- O—Wrapping for electrical insulation (mica is suggested)
- P—Refractory cement

NOTE—A steel alloy, such as Inconel X, may be used as an alternative in place of copper and will allow measurements at higher temperatures.

FIG. 1 Apparatus for Determination of Annealing Point and Strain Point of Glass