



Designation: D6635 – 15

Standard Test Method for Performing the Flat Plate Dilatometer¹

This standard is issued under the fixed designation D6635; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

1. Scope*

1.1 This test method describes an in-situ penetration plus expansion test. The test is initiated by forcing the steel, flat plate, dilatometer blade², with its sharp cutting edge, into a soil. Each test consists of an increment of penetration, generally vertical, followed by the expansion of a flat, circular, metallic membrane into the surrounding soil. The test provides information about the soil's in-situ stratigraphy, stress, strength, compressibility, and pore-water pressure for use in the design of earthworks and foundations.

1.2 This method includes specific requirements for the preliminary reduction of dilatometer test data. It does not specify how to assess or use soil properties for engineering design.

1.3 This method applies best to those sands, silts, clays, and organic soils that can be readily penetrated with the dilatometer blade, preferably using static push (see 4.2). Test results for soils containing primarily gravel-sized particles and larger may not be useful without additional research.

1.4 This method is not applicable to soils that cannot be penetrated by the dilatometer² blade without causing significant damage to the blade or its membrane.

1.5 The text of this standard references notes and footnotes that provide explanatory material. These notes and footnotes shall not be considered as requirements of the standard. The illustrations included in this standard are intended only for explanatory or advisory use

1.6 *Units*—The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard. Reporting of test results in units other than SI shall not be regarded as nonconformance with this test method

¹ This test method is under the jurisdiction of ASTM Committee D18 on Soil and Rock and is the direct responsibility of Subcommittee D18.02 on Sampling and Related Field Testing for Soil Evaluations.

Current edition approved Nov. 1, 2015. Published December 2015. Originally approved in 2001. Last previous edition approved in 2007 as D6635 – 01(2007). DOI: 10.1520/D6635-15.

² The dilatometer is covered by a patent. Interested parties are invited to submit information regarding the identification of an acceptable alternative(s) to this patented item to the ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend.

1.7 All observed and calculated values shall conform to the guidelines for significant digits and rounding established in Practice D6026.

1.8 The procedures used to specify how data are collected/recorded and calculated in this standard are regarded as the industry standard. In addition, they are representative of the significant digits that should generally be retained. The procedures used do not consider material variation, purpose for obtaining the data, special purpose studies, or any considerations for the user's objectives; and it is common practice to increase or reduce significant digits of reported data to commensurate with these considerations. It is beyond the scope of this standard to consider significant digits used in analysis methods for engineering design.

1.9 ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

1.10 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards*:³

- D653 Terminology Relating to Soil, Rock, and Contained Fluids
- D1586 Test Method for Penetration Test (SPT) and Split-Barrel Sampling of Soils
- D2435 Test Methods for One-Dimensional Consolidation Properties of Soils Using Incremental Loading
- D3441 Test Method for Mechanical Cone Penetration Tests of Soil (Withdrawn 2014)⁴

³ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

⁴ The last approved version of this historical standard is referenced on www.astm.org.

*A Summary of Changes section appears at the end of this standard

- D3740** Practice for Minimum Requirements for Agencies Engaged in Testing and/or Inspection of Soil and Rock as Used in Engineering Design and Construction
- D5778** Test Method for Electronic Friction Cone and Piezocone Penetration Testing of Soils
- D6026** Practice for Using Significant Digits in Geotechnical Data

3. Terminology

3.1 Definitions:

3.1.1 For definitions of common technical terms in this standard, refer to Terminology **D653**.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *A-pressure*—the gauge gas pressure against the inside of the membrane when the center of the membrane has lifted above its support and moved laterally 0.05-mm (tolerance +0.02, -0.00 mm) into the soil surrounding the blade.

3.2.2 *B-pressure*—the gauge gas pressure against the inside of the membrane when the center of the membrane has lifted above its support and moved laterally 1.10-mm (± 0.03 mm) into the soil surrounding the blade.

3.2.3 *C-pressure*—The gauge gas pressure against the inside of the membrane when the center of the membrane returns to the *A-pressure* position during a controlled, gradual deflation following the *B-pressure*.

3.2.4 *dilatometer sounding*—the entire sequence of dilatometer tests along a vertical line of penetration in the soil.

3.2.5 *dilatometer test (DMT)*—the complete procedure of penetration, membrane inflation and then deflation for a single test depth using the flat plate dilatometer.

3.2.6 *membrane*—a thin, flexible, 60-mm diameter circular piece of sheet metal (usually stainless steel), fixed around its edges, that mounts on one side of the dilatometer blade and which, as a result of an applied internal gas pressure, expands into the soil in an approximate spherical shape along an axis perpendicular to the plane of the blade.

3.3 Symbols:

3.3.1 ΔA —the gauge gas pressure inside the membrane (corrected for Z_m) required to overcome the stiffness of the membrane and move it inward to a center-expansion of 0.05 mm (a negative gauge or suction pressure, but recorded as positive) with only ambient atmospheric pressure acting externally.

3.3.2 ΔB —the gauge gas pressure inside the membrane (corrected for Z_m) required to overcome the stiffness of the membrane and move it outward to a center-expansion of 1.10 mm against only the ambient atmospheric pressure.

3.3.3 E_D —the dilatometer modulus, based on linear elastic theory, and the primary index used in the correlation for the constrained and Young's moduli (see Section 10).

3.3.4 G_m —bulk specific gravity = moist soil unit weight divided by the unit weight of water.

3.3.5 I_D —the dimensionless dilatometer material index, used to identify soil type and delineate stratigraphy (see Section 10).

3.3.6 K_D —the dimensionless dilatometer horizontal stress index, the primary index used in the correlation for in-situ horizontal stress, overconsolidation ratio, and undrained shear strength in cohesive soils. K_D is similar to the at-rest coefficient of earth pressure except that it includes blade penetration effects.

3.3.7 P —the total push, or thrust force required to advance only the dilatometer blade to its test depth, measured at its test depth and exclusive of soil or other friction along the pushrods.

3.3.8 p_o —the *A-pressure* reading, corrected for Z_m , the ΔA membrane stiffness at 0.05-mm expansion, and the 0.05-mm expansion itself, to estimate the total soil stress acting normal to the membrane immediately before its expansion into the soil (0.00-mm expansion, see Section 10).

3.3.9 p_I —the *B-pressure* reading corrected for Z_m and the ΔB membrane stiffness at 1.10-mm expansion to give the total soil stress acting normal to the membrane at 1.10-mm membrane expansion (see Section 10).

3.3.10 p_2 —The *C-pressure* reading corrected for Z_m and the ΔA membrane stiffness at 0.05-mm expansion and used to estimate pore-water pressure (see 10.3).

3.3.11 σ'_v —vertical effective stress at the center of the membrane before the insertion of the DMT blade.

3.3.12 σ_v —total vertical stress at the center of the membrane before the insertion of the DMT blade, generally calculated from unit weights estimated using the DMT results.

3.3.13 u_o —the pore-water pressure acting at the center of the membrane before the insertion of the DMT blade (often assumed as hydrostatic below the water table surface).

3.3.14 Z_m —the gauge pressure deviation from zero when vented to atmospheric pressure (an offset used to correct pressure readings to the true gauge pressure).

4. Summary of Test Method

4.1 A dilatometer test (DMT) consists of forcing the dilatometer blade into the soil, with the membrane facing the horizontal direction, to a desired test penetration, measuring the thrust to accomplish this penetration and then using gas pressure to expand a circular steel membrane located on one side of the blade. The operator measures and records the pressure required to produce expansion of the membrane into the soil at two preset deflections. The operator then deflates the membrane, possibly recording an optional third measurement, advances the blade the desired penetration increment and repeats the test. Each test sequence typically requires about two minutes. A dilatometer sounding consists of the results from all the tests at one location presented in a fashion indicating variation with depth.

4.2 The operator may advance the blade using either a quasi-static push force or dynamic impact from a hammer, with quasi-static push preferred. A record of the penetration resistance (thrust force or blows per penetration increment) is desirable both for control of the penetration and later analyses.

NOTE 1—In soils sensitive to impact and vibrations, such as medium to loose sands or sensitive clays, dynamic insertion methods can significantly change the test results compared to those obtained using a quasi-static

push. In general, structurally sensitive soils will appear more compressible when tested using dynamic insertion methods. In such cases check for dynamic effects and, if important, calibrate and adjust test interpretations accordingly.

4.3 The penetration increment typically used in a DMT sounding varies from 0.15 to 0.30 m. Most soundings are performed vertically and this Test Method requires that the membrane face the horizontal direction. Testing below impenetrable layers will require preboring and supporting (if required) a borehole with a diameter of at least 100 mm.

4.4 The operator performs a membrane calibration before and after each DMT sounding.

4.5 The field data is then interpreted to obtain profiles of those engineering soil properties of interest over the depth range of the DMT sounding.

5. Significance and Use

5.1 Soundings performed using this test method provide a detailed record of dilatometer results, which are useful for evaluation of site stratigraphy, homogeneity, depth to firm layers, voids or cavities, and other discontinuities. The penetration resistance, if obtained, and subsequent membrane expansion are used for soil classification and correlation with the engineering properties of soils.

5.2 The DMT may provide measurements of penetration resistance, lateral stress, deformation modulus, and pore-water pressure (in sands). However, the in-situ soil properties are affected by the penetration of the blade. Therefore, published correlations are used to estimate soil properties for the design and construction of earthworks and foundations for structures, and to predict the behavior of soils subjected to static or dynamic loads.

5.3 This test method tests the soil in-situ and soil samples are not obtained. However, the interpretation of the results from this test method does provide an estimate of the types of

soil penetrated. Soil samples from parallel borings may be obtained for correlation purposes, but prior information or experience may preclude the need for borings.

NOTE 2—The quality of the result produced by this test method is dependent on the competence of the personnel performing it, and the suitability of the equipment and facilities used. Agencies that meet the criteria of Practice D3740 are generally considered capable of competent and objective testing/sampling/ inspection/etc. Users of this test method are cautioned that compliance with Practice D3740 does not in itself assure reliable results. Reliable results depend on many factors; Practice D3740 provides a means of evaluating some of those factors.

6. Apparatus

6.1 The annotated Fig. 1 illustrates the major components of the DMT equipment, exclusive of that required to insert the blade. The equipment dimensions, tolerances, deflections, etc. affect the test results and shall conform to the values provided herein.

6.1.1 *Blade*, (1), 96 mm wide (95 to 97 mm) and 15 mm thick (13.8 to 15 mm).

6.1.2 *Membrane*, (2), 60 mm diameter.

6.1.3 *Control Unit*, with a pressure readout system (3) that can vary in type, range, and sensitivity as required. The pressure readout system shall have an accuracy of 0.5 percent of span or better (0.25 percent of span is recommended). The unit shown has both low-range and high-range Bourdon gauges that are read manually. Older units have a single Bourdon gauge, typically medium-range. The gauges should be annually calibrated against a traceable standard, more often if heavily used. The control unit also includes connections (5) for a pressure source, a pneumatic-electrical cable, and an electrical ground cable, and has valves to control gas flow and vent the system (6).

6.1.4 *Calibration Syringe*, (4) for determining the ΔA and ΔB membrane calibrations using the low-range Bourdon gauge. Some control units have a separate low-range pressure

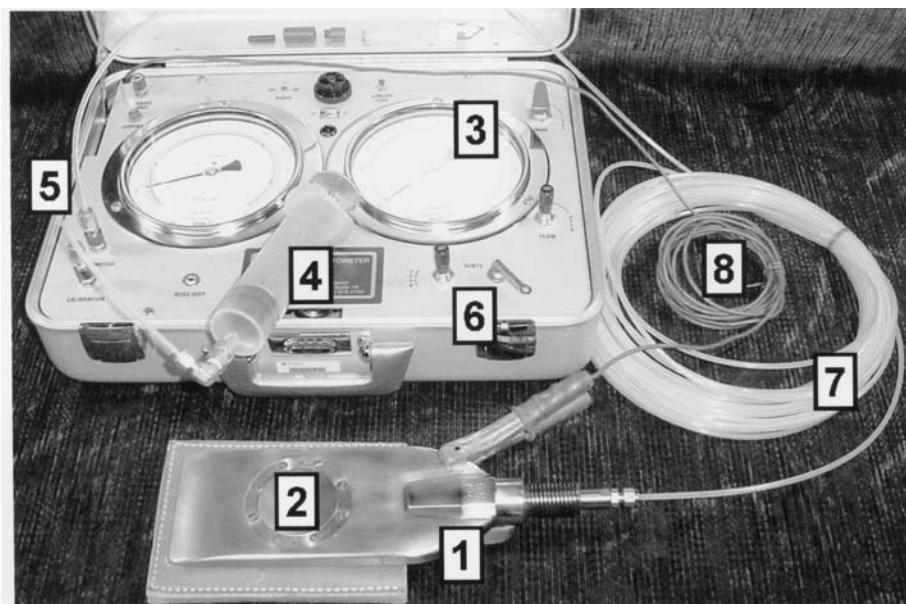


FIG. 1 DMT Equipment

gauge that attaches to the control unit for determining the ΔA and ΔB membrane calibrations

6.1.5 *Pneumatic-Electrical Cable*, (7) to transmit gas pressure and electrical continuity from the control unit to the blade.

6.1.6 *Ground Cable*, (8) to provide electrical continuity between the push rod system and the calibration unit.

6.2 Insertion equipment is required to advance the blade to the test depth. The blade may be pushed using the quasi-static thrust of a drill rig or cone penetrometer rig (CPT, see Test Method [D3441](#), [D5778](#)), driven using a hammer such as in the standard penetration test (SPT, see Test Method [D1586](#) and [Note 1](#)), or inserted using other suitable equipment. Drill rig support may be required to bore through impenetrable soil or rock layers above the desired test depth.

6.3 Push rods are required to transfer the thrust from the surface insertion equipment and to carry the pneumatic-electrical cable from the surface control unit to the dilatometer blade. The rods are typically those used with the CPT (Test Method [D3441](#), [D5778](#)) or SPT (Test Method [D1586](#)) equipment. Suitable adapters are required to attach the blade to the bottom of the rod string and allow the cable to exit near the top of the rods. When testing from the bottom of a borehole, the cable may exit from the rod string some suitable distance above the blade and then be taped to the outside of the rods at appropriate intervals. The exposed cable should not be pinched or allowed to penetrate the soil.

6.4 A gas pressure tank with a suitable regulator and tubing to connect it to the control unit is required. The operator may use any nonflammable, noncorrosive, nontoxic gas as a pressure source. Dry nitrogen is recommended.

6.5 A suitable load cell, just above the blade (preferred) or at the top of the rods, is required to measure the thrust P applied during the blade penetration. Hydraulic ram pressure may also be used to measure thrust with proper correlation. Parasitic soil-rod friction is generally insignificant in sands, but may be measured during upward withdrawal. Load cells shall have an accuracy of 0.5 kN or better.

7. Interferences

7.1 *Timely Readings*—Experiments have determined that testing within the time limits of [9.2.3](#) results in essentially drained conditions in sands and undrained conditions in clays and that the results are not sensitive to time-for-reading changes by a factor of 2. However, in saturated silty soils and sand/clay mixtures with intermediate permeabilities, partially drained conditions probably exist, and the results and correlations depend more importantly on the use of proper time intervals. Unsaturated soils are believed to behave in an approximately drained fashion.

7.2 *Rate of Pressurization*—Since very little membrane movement occurs before the A -pressure, the operator may reduce testing time by initially pressurizing at a rapid rate, then slowing to accurately read the A -pressure. This technique has minimal effect on the A -pressure measurement but does risk a poor reading if it occurs unexpectedly. A steady, readable rate is preferred for the pressure increment from the A - to B -pressure. Check the chosen flow rate by closing the flow

control valve during the test and observing the gauge for a drop in pressure before stabilizing. If the pressure drops in excess of 2 percent, the rate is too fast. Longer cables require a slower flow rate for accurate readings.

7.3 *Weak Soils*—Accurate, timely readings are very important when testing soft or weak soils. Also at shallow depths in very weak (or partially saturated soils), the lateral soil pressure may not exceed the ΔA membrane stiffness to produce the required initial signal. For sensitive testing of this type, choose a membrane with low and consistent calibration values. As an alternative, before advancing to the test depth, close the vent valve, use the calibration syringe to collapse the membrane with an initial suction or vacuum, and then remove the syringe leaving the negative pressure locked in. After advancing the blade with the membrane collapsed, read the A -pressure as in [9.2.3](#), recording vacuum as a negative value. The calibration unit can also be used to apply the initial vacuum, but it cannot be removed until reading zero pressure during the test. Alternatively, bypass shallow testing until reaching a depth that produces the initial signal.

7.4 *Membrane Damage*—Damage to the membrane typically occurs when brushing against or pushing through gravel, large shells, unweathered rock, concretions, miscellaneous fill, and buried obstructions. In soils containing such obstacles be alert for membrane malfunction. Continued usage in highly abrasive soils, such as dense quartz sands, gradually wears down blades and membranes and makes them more susceptible to further damage. Replace membranes when wear or wrinkling inhibits the smooth expansion of the membrane or will likely cause rupture during penetration.

7.5 *Blade Damage*—Bending of the blade, excessive wear and wrinkling of the cutting edge typically occur when a high penetration thrust P is required such as in hard clays or dense sands, especially with gravel, large shells, unweathered rock, cementations and similar inclusions. The probability of damage is significant above a thrust of approximately 45 kN and very high above 90 kN. Users have successfully performed soundings in strong soils with thrust exceeding 180 kN. However, a lack of lateral support for the push rods above the ground surface, or in weak soil layers above the blade, may lead to a buckling failure of the push rods, rod adapter, or blade at thrust values less than 45 kN. The user incurs a greater risk of damage when applying a high penetration thrust and should remain vigilant for indications of damage.

7.6 *Rotary Drilling Equipment*—The blade and its connections are not designed for high torsion forces. Make all rod connections using no more torsion than produced by hand wrench tightening. Do not allow the making of connections with the aid of engine power.

7.7 *Verticality*—The dilatometer blade may drift out of plumb when inserted with initial horizontal forces acting, when penetrating soils with inclusions (see [7.5](#)) or when encountering obstructions. The deeper the sounding the more likely that appreciable deflection may occur. With usual care this problem is not significant in ordinary sands and clays for sounding depths of less than 15 m. However, be alert for indications of drift, such as unusual “crunching” sounds, out of plumb rods,

suspicious data, or specific soil layers encountered deeper than expected. Research indicates no significant effect on the test results for soundings performed within 15 degrees of the vertical axis.

7.8 Leak Checks During Sounding—Periodically check for any leaks in the lines or connections by momentarily closing the control valve during the interval between the *A*- and *B*-pressures. If the pressure remains constant, then the system has no leaks, as required. Identify the source of any leaks before continuing the sounding. Control unit leakage greater than 100 kPa/min and any leaks in the blade or cable must be repaired before continuing. In the event that subsurface leakage forces termination of a sounding, maintain a pressure in the system of 100 to 200 kPa above u_0 while withdrawing the blade to prevent entry of soil and water.

7.9 Prompt Readings—Make all gauge readings promptly and accurately. In very noisy testing environments or poor electrical grounding conditions it may be difficult to hear the audio signal that prompts and *A*- and *B*-pressure readings. In this case, use either a visual cue on the control unit or an earphone to insure timely detection of the audio signal.

7.10 Electrical Short—If the electric audio signal does not cease at a reasonable *A*-pressure (based on previous readings and thrust measurements), then a short circuit is likely. Possible causes include a poorly connected cable (especially at the blade), entry of soil or water into the cable through a torn tubing or loose fitting, or infiltration of soil or water into the blade, especially through a ruptured membrane. Locate and correct the short before continuing the sounding.

7.11 Electrical Discontinuity—If the electric audio signal does not initiate when penetrating to the test depth, or does not return at a reasonable *B*-pressure (based on previous readings and thrust measurements), then a discontinuity is possible in the electrical circuit to, from or within the blade. (See section 7.3 also.) Over-expansion of the membrane and unacceptable changes in the membrane calibrations may result if the *B*-pressure is exceeded. Soil inside the blade may interfere with the electrical switching and cause this problem. Locate and correct the discontinuity before continuing the sounding.

7.12 Nearby Soundings and Borings—DMT soundings should not be performed within the zone of soil affected by another sounding or boring. Good test practice requires a minimum clear distance of 1.0 m from an existing CPT sounding (Test Method **D3441**, **D5778**) and 25 boring diameters from an existing, unbackfilled or uncased boring. Increase these/distances if the sounding or boring logs include significant lateral drift, borehole collapse or loss of circulation. If possible, complete the DMT soundings before any borings.

7.13 Borings Used to Advance DMT Soundings—When dilatometer tests are performed below a borehole, disregard any DMT results within the zone of disturbance at the hole bottom, typically three to five borehole diameters. Casing or drilling mud or both should be used to stabilize borings in saturated soils, and drill fluid should be maintained above the ground water surface at all times. Bottom discharge drill bits are not permissible for advancing DMT soundings.

8. Hazards

8.1 The following safety recommendations are in addition to general safety requirements applicable to construction operations: (Also see 1.10.)

8.2 Permit only authorized personnel within the immediate test area, and only as necessary to operate test equipment.

8.3 Provide a stable and level work area around the thrust machine. Keep all test and adjacent work areas, walkways, platforms, etc. clear of scrap, debris, small tools, and accumulations of snow, ice, mud, grease, oil, or other slippery substances.

8.4 Carry out all operations in connection with dilatometer penetration in a manner that minimizes, avoids, or eliminates the exposure of people to hazard. Test personnel should wear safety glasses, gloves, safety shoes, and appropriate hearing protection.

8.5 Be aware of and avoid pinch and crush hazards while using thrust equipment.

8.6 The application of thrust to the penetration rods can result in damage to equipment and hazard to personnel. The applied thrust at which rods may break is a function of the rod design, the thrust equipment configuration, and the ground conditions. Standard push rods can be damaged or broken at loads less than their rated capacity. The amount of force that push rods are able to sustain decreases as the unrestrained rod length increases. Push rod joints and push rod-penetrometer tip connections provide weak links in the rod string. Excessive lateral rod deflection is the most common cause for rod breakage.

8.7 Inspect pressure hoses and connections for damage before, during, and after usage. Do not pressurize dilatometer components beyond manufacturer recommendations.

9. Procedure

9.1 Preparation for Testing and Calibration:

9.1.1 Select for testing only blades that conform to the manufacturer's internal tolerance adjustments and that are in good visual external condition. The blade should have no discernible bend, defined as a clearance of 0.5 mm or more under a 150-mm straight edge placed along the blade parallel to its axis. Its penetrating edge should be straight and sharp, and it should not deviate more than 2 mm transverse to the axis of the rods.

9.1.2 Attach the pressure source and pneumatic-electrical cable to the control unit. Plug the blade end of the cable with an appropriate fitting and apply 4-6 MPa pressure to the cable through the control unit. Close the flow control valve and observe the gauge for any pressure drop that would indicate a leak in the system. Locate and repair any leaks in the cable. Small leaks (less than 100 kPa/min) in the control unit, though undesirable and indicative of a potential problem, should not significantly affect the test results.

9.1.3 Thread the pneumatic-electrical cable through the lower blade-rod adapter, as many of the push rods as needed and any other adapters, stabilizers or push frames as required. Always cap the cable ends to prevent contamination of the

cables and corrosion of the terminals. Connect and tighten the cable to the blade. Insure that the blade and any lower adapters shoulder squarely and tightly to the bottom rod.

9.1.4 Attach the pneumatic-electrical cable to the control unit and connect the ends of the electrical ground cable to the control unit and blade, respectively. To check the circuitry, press the center of the membrane down to activate the electrical/audio signal on the control unit.

9.1.5 With the membrane unrestrained, use the calibration equipment to determine and record the ΔA and ΔB membrane stiffness pressures with a precision of 1 kPa. Correct the ΔA and ΔB for the gauge offset, Z_m . The calibrations should fall within the manufacturer tolerances and are recorded as positive values. The electrical/audio signal should stop and start unambiguously at the 0.05-mm and 1.10-mm expansions. The membrane should be free of wrinkles and deep scratches and should expand smoothly during pressurization without popping or snapping sounds. Repeat the calibration procedure several times to verify consistency. Replace any membrane that fails these checks.

9.1.6 The calibration procedure provides a final check of the equipment prior to testing. If the equipment is disassembled for any reason, the operator should verify the calibrations before proceeding.

9.2 DMT Procedure:

9.2.1 With the vent valve open and the push rods vertical, advance the dilatometer blade to the first depth. Advance the blade by means of quasi-static push at a rate of 10-30 mm/sec. If possible, measure and record the thrust just before reaching the test depth with a precision of 0.5 kN or better. An example field data sheet is shown in Fig. X1.2. Alternatively advance the blade using a drop hammer and record the number of blows required for each 0.10-0.15 m of penetration. If estimating the equivalent static thrust from blow counts, use an average of above and below the test depth. Borehole predrilling with casing or drilling mud is acceptable as required.

9.2.2 The blade penetration must produce an electrical/audio signal to indicate the membrane has been pressed flush against the blade to start the 9.2.3 DMT sequence. See 7.3.

9.2.3 Within 15 seconds after reaching the test depth, unload any static force on the push rods, close the vent valve, and pressurize the membrane. The gauge pressure at the instant the electrical/audio signal stops (0.05-mm membrane displacement) is recorded as the *A*-pressure reading. Obtain this reading within 15 to 30 seconds after beginning the gas flow. Without stopping the gas flow at the *A*-pressure, continue pressurization of the membrane until the signal comes on again at a 1.10-mm displacement. This is the *B*-pressure reading and should be obtained 15 to 30 seconds after beginning the gas flow. These time limits require that the pressurization rate be varied according to the anticipated pressure readings, faster in stiff soils and dramatically slower in soft soils. Record pressure readings with the best possible precision, typically 1 kPa for a low-range gauge (up to 1 MPa) and 5 to 10 kPa for a high-range gauge. Upon reaching the *B*-pressure, immediately open the vent valve and stop the gas flow. Immediate depressurization prevents over-expansion of the membrane, which may change its calibrations. See 9.2.4 for an alternative,

controlled depressurization procedure to obtain the “*C*-pressure” (strongly recommended). If pressurization is stopped prior to obtaining the *B*-pressure, note the maximum pressure applied as a deviation.

NOTE 3—The difference between the *A*-pressure and *B*-pressure readings should always be greater than the sum of the ΔA and ΔB calibrations.

9.2.4 At least every other dilatometer test in a sounding (preferably more) should include a smooth, controlled depressurization to measure the *C*-pressure. A flow-control vent valve should be used for this purpose. Read the *C*-pressure on the low-range gauge when the membrane has deflated to the *A*-pressure position (0.05-mm deflection) and the electric signal comes on again (not when the *B*-pressure signal stops). Obtain and record the *C*-pressure to the nearest 1 kPa within 15 to 30 seconds immediately following the *B*-pressure.

NOTE 4—The pore-water pressure must exceed the ΔA calibration to result in a positive *C*-pressure reading. If the electric signal does not activate during the *C*-pressure deflation then use the calibration syringe to apply a suction and obtain a negative *C*-pressure. The value of p_2 will remain positive provided the magnitude of the negative *C*-pressure does not exceed the ΔA calibration (see Table 1).

NOTE 5—The *C*-pressure is sensitive to operator technique. Abrupt pressure changes during the membrane deflation may collapse the soil in front of the membrane and yield a poor measurement. In free-draining soils, the *C*-pressure will not change significantly with time and the operator may check it by repeating the (A-B-C) sequence. The *A*- and *B*-pressures will change from the initial test but the *C*-pressure should remain constant. The repeated *A*- and *B*-pressures are not generally useful. Soils that are not freely-drained will behave differently (see 9.3).

9.2.5 Repeat the test sequence for a new set of *A*-, *B*-, and possibly *C*-pressures, at each depth interval down to the maximum depth of the sounding. The minimum penetration increment between tests is 100 mm. Pressure check the system every third or fourth test during the sounding. See 7.8 for details.

9.3 *A*-Pressure Dissipation Tests (optional):

9.3.1 In poorly drained soils, with $I_D < 2$, the excess pore-water pressure induced by the blade penetration usually dissipates over a period of time longer than required for a dilatometer test. The coefficient of consolidation may be estimated by observing the dissipation of the *A*-pressure. To perform a dissipation test, stop the blade penetration at the chosen test depth and make successive *A*-pressure readings over time. Dissipation tests can be time consuming and are performed only as needed. Two similar test procedures, the A_2 -method and the *A*-method, are described in 9.3.2 and 9.3.3 respectively. Either is acceptable.

NOTE 6—Before making a detailed analysis of the time-dissipation curves in 9.3.2 and 9.3.3, the *A*-pressure measurements may be corrected to obtain p_0 values. If a paired *B*-pressure measurement is available, as for the final *A*-pressure, then p_0 may be calculated as shown in Table 1. For dissipation analysis a paired *B*-pressure is generally not available, and the following equation may be used to correct *A*-pressure readings:

$$p_0 (\text{dissipation}) = (A - Z_m + \Delta A)$$

9.3.2 *A*₂-method Dissipation—This procedure attempts to measure the pore-water pressure directly and determine consolidation parameters from analysis of the resulting pore-pressure curve. The A_2 -method requires a complete dilatometer test (A-B-C) before beginning a series of *A*-pressure only