



Designation: E797/E797M – 15

# Standard Practice for Measuring Thickness by Manual Ultrasonic Pulse-Echo Contact Method<sup>1</sup>

This standard is issued under the fixed designation E797/E797M; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope\*

1.1 This practice<sup>2</sup> provides guidelines for measuring the thickness of materials using the contact pulse-echo method at temperatures not to exceed 93°C [200°F].

1.2 This practice is applicable to any material in which ultrasonic waves will propagate at a constant velocity throughout the part, and from which back reflections can be obtained and resolved.

1.3 *Units*—The values stated in either SI units or inch-pound units are to be regarded separately as standard. The values stated in each system may not be exact equivalents; therefore, each system shall be used independently of the other. Combining values from the two systems may result in non-conformance with the standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

## 2. Referenced Documents

2.1 *ASTM Standards*:<sup>3</sup>

- E317 Practice for Evaluating Performance Characteristics of Ultrasonic Pulse-Echo Testing Instruments and Systems without the Use of Electronic Measurement Instruments
- E494 Practice for Measuring Ultrasonic Velocity in Materials
- E543 Specification for Agencies Performing Nondestructive Testing
- E1316 Terminology for Nondestructive Examinations

<sup>1</sup> This practice is under the jurisdiction of ASTM Committee E07 on Nondestructive Testing and is the direct responsibility of Subcommittee E07.06 on Ultrasonic Method.

Current edition approved Dec. 1, 2015. Published December 2015. Originally approved in 1981. Last previous edition approved in 2010 as E797 - 10. DOI: 10.1520/E0797\_E0797M-15.

<sup>2</sup> For ASME Boiler and Pressure Vessel Code applications, see related Practice SE-797 in Section II of that Code.

<sup>3</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

2.2 *ASNT Documents*:<sup>4</sup>

- Nondestructive Testing Handbook, 2nd Edition, Vol 7*
- SNT-TC-1A Recommended Practice for Personnel Qualification and Certification in Nondestructive Testing
- ANSI/ASNT CP-189 Standard for Qualification and Certification of Nondestructive Testing Personnel

2.3 *Aerospace Industries Association Document*:<sup>5</sup>

- NAS-410 Certification and Qualification of Nondestructive Testing Personnel

2.4 *ISO Standard*:<sup>6</sup>

- ISO 9712 Non-Destructive Testing—Qualification and Certification of NDT Personnel

## 3. Terminology

3.1 *Definitions: Definitions*—For definitions of terms used in this practice, refer to Terminology E1316.

## 4. Summary of Practice

4.1 Thickness ( $T$ ), when measured by the pulse-echo ultrasonic method, is a product of the velocity of sound in the material and one half the transit time (round trip) through the material.

$$T = \frac{Vt}{2}$$

where:

- $T$  = thickness,
- $V$  = velocity, and
- $t$  = transit time.

4.2 The pulse-echo ultrasonic instrument measures the transit time of the ultrasonic pulse through the part.


4.3 The velocity in the material being examined is a function of the physical properties of the material. It is usually assumed to be a constant for a given class of materials. Its approximate value can be obtained from Table X3.1 in Practice

<sup>4</sup> Available from American Society for Nondestructive Testing (ASNT), P.O. Box 28518, 1711 Arlingate Ln., Columbus, OH 43228-0518, http://www.asnt.org.

<sup>5</sup> Available from Aerospace Industries Association of America, Inc. (AIA), 1000 Wilson Blvd., Suite 1700, Arlington, VA 22209-3928, http://www.aia-aerospace.org.

<sup>6</sup> Available from International Organization for Standardization (ISO), ISO Central Secretariat, BIBC II, Chemin de Blandonnet 8, CP 401, 1214 Vernier, Geneva, Switzerland, http://www.iso.org.

\*A Summary of Changes section appears at the end of this standard

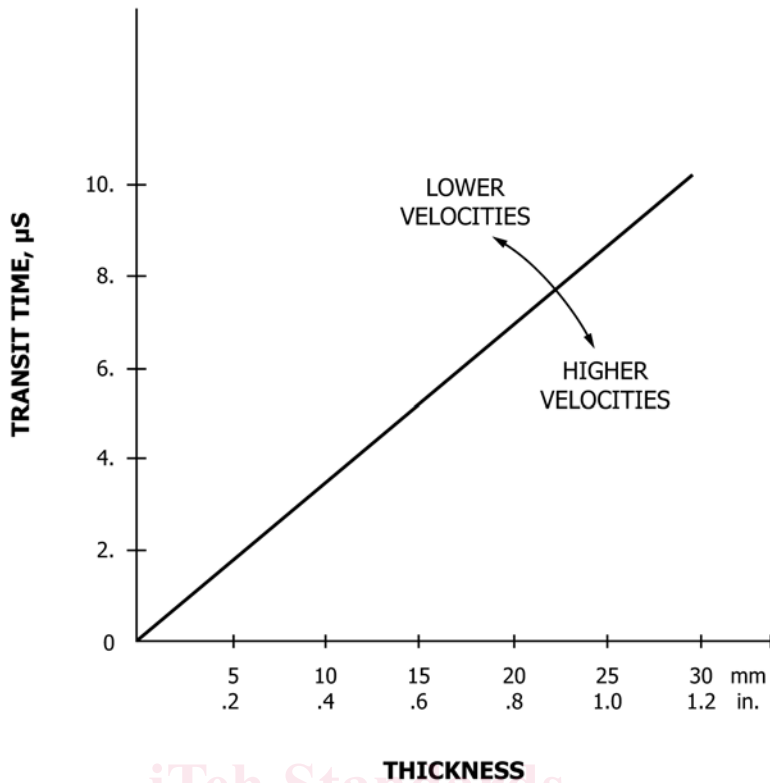

NOTE 1—Slope of velocity conversion line is approximately that of steel.

FIG. 1 Transit Time/Thickness Relationship

E494 or from the *Nondestructive Testing Handbook*, or it can be determined empirically.

4.4 One or more reference blocks are required having known velocity, or of the same material to be examined, and having thicknesses accurately measured and in the range of thicknesses to be measured. It is generally desirable that the thicknesses be “round numbers” rather than miscellaneous odd values. One block should have a thickness value near the maximum of the range of interest and another block near the minimum thickness.

4.5 The display element (A-scan display, meter, or digital display) of the instrument must be adjusted to present convenient values of thickness dependent on the range being used. The control for this function may have different names on different instruments, including *range*, *sweep*, *material standardize*, or *velocity*.

4.6 The timing circuits in different instruments use various conversion schemes. A common method is the so-called time/analog conversion in which the time measured by the instrument is converted into a proportional d-c voltage which is then applied to the readout device. Another technique uses a very high-frequency oscillator that is modulated or gated by the appropriate echo indications, the output being used either directly to suitable digital readouts or converted to a voltage for other presentation. A relationship of transit time versus thickness is shown graphically in Fig. 1.

## 5. Significance and Use

5.1 The techniques described provide indirect measurement of thickness of sections of materials not exceeding temperatures of 93°C [200°F]. Measurements are made from one side of the object, without requiring access to the rear surface.

5.2 Ultrasonic thickness measurements are used extensively on basic shapes and products of many materials, on precision machined parts, and to determine wall thinning in process equipment caused by corrosion and erosion.

5.3 Recommendations for determining the capabilities and limitations of ultrasonic thickness gages for specific applications can be found in the cited references.<sup>7,8</sup>

## 6. Basis of Application

6.1 The following items are subject to contractual agreement between the parties using or referencing this practice.

### 6.2 Personnel Qualification:

6.2.1 If specified in the contractual agreement, personnel performing examinations to this standard shall be qualified in accordance with a nationally or internationally recognized

<sup>7</sup> Bosselaar, H., and Goosens, J.C.J., “Method to Evaluate Direct-Reading Ultrasonic Pulse-Echo Thickness Meters,” *Materials Evaluation*, March 1971, pp. 45–50.

<sup>8</sup> Fowler, K.A., Elfbaum, G.M., Husarek, V., and Castel, J., “Applications of Precision Ultrasonic Thickness Gaging,” *Proceedings of the Eighth World Conference on Nondestructive Testing*, Cannes, France, Sept. 6–11, 1976, Paper 3F5.

NDT personnel qualification practice or standard such as ANSI/ASNT CP-189, SNT-TC-1A, NAS-410, ISO 9712, or a similar document and certified by the employer or certifying agency, as applicable. The practice or standard used and its applicable revision shall be identified in the contractual agreement between the using parties.

**6.3 Qualification of Nondestructive Agencies**—If specified in the contractual agreement, NDT agencies shall be qualified and evaluated as described in Specification E543. The applicable edition of Specification E543 shall be specified in the contractual agreement.

**6.4 Procedures and Techniques**—The procedures and techniques to be utilized shall be as specified in the contractual agreement.

**6.5 Surface Preparation**—The pre-examination surface preparation criteria shall be specified in the contractual agreement.

## 7. Apparatus

**7.1 Instruments**—Thickness-measurement instruments are divided into three groups: (1) Flaw detectors with an A-scan display readout, (2) Flaw detectors with an A-scan display and direct thickness readout, and (3) Direct thickness readout.

**7.1.1** Flaw detectors with A-scan display readouts display time/amplitude information. Thickness determinations are made by reading the distance between the zero-corrected initial pulse and first-returned echo (back reflection), or between multiple-back reflection echoes, on a standardized base line of the A-scan display. The base line of the A-scan display should be adjusted for the desired thickness increments.

**7.1.2** Flaw detectors with numeric readout are a combination pulse ultrasound flaw detection instrument with an A-scan display and additional circuitry that provides digital thickness information. The material thickness can be electronically measured and presented on a digital readout. The A-scan display provides a check on the validity of the electronic measurement by revealing measurement variables, such as internal discontinuities, or echo-strength variations, which might result in inaccurate readings.

**7.1.3** Thickness readout instruments are modified versions of the pulse-echo instrument. The elapsed time between the initial pulse and the first echo or between multiple echoes is converted into a meter or digital readout. The instruments are designed for measurement and direct numerical readout of specific ranges of thickness and materials.

**7.2 Search Units**—Most pulse-echo type search units (straight-beam contact, delay line, and dual element) are applicable if flaw detector instruments are used. If a thickness readout instrument has the capability to read thin sections, a highly damped, high-frequency search unit is generally used. High-frequency (10 MHz or higher) delay line search units are generally required for thicknesses less than about 0.6 mm [0.025 in.]. Measurements of materials at high temperatures require search units specially designed for the application. When dual element search units are used, their inherent nonlinearity usually requires special corrections for thin sec-

tions. (See Fig. 2.) For optimum performance, it is often necessary that the instrument and search units be matched.

**7.3 Standardization Blocks**—The general requirements for appropriate standardization blocks are given in 4.4, 8.1.3, 8.2.2.1, 8.3.2, and 8.4.3. Multi-step blocks that may be useful for these standardization procedures are described in Appendix X1 (Figs. X1.1 and X1.2).

## 8. Standardization of Apparatus

**8.1 Case I—Direct Contact, Single-Element Search Unit:**

**8.1.1 Conditions**—The display start is synchronized to the initial pulse. All display elements are linear. Full thickness is displayed on the A-scan display.

**8.1.2** Under these conditions, we can assume that the velocity conversion line effectively pivots about the origin (Fig. 1). It may be necessary to subtract the wear-plate time, requiring minor use of delay control. It is recommended that standardization blocks providing a minimum of two thicknesses that span the thickness range be used to check the full-range accuracy.

**8.1.3** Place the search unit on a standardization block of known thickness with suitable couplant and adjust the instrument controls (material standardization, range, sweep, or velocity) until the display presents the appropriate thickness reading.

**8.1.4** The readings should then be checked and adjusted on standardization blocks with thickness of lesser value to improve the overall accuracy of the system.

**8.2 Case II—Delay Line Single-Element Search Unit:**

**8.2.1 Conditions**—When using this search unit, it is necessary that the equipment be capable of correcting for the time during which the sound passes through the delay line so that the end of the delay can be made to coincide with zero thickness. This requires a so-called “delay” control in the instrument or automatic electronic sensing of zero thickness.

**8.2.2** In most instruments, if the material standardize circuit was previously adjusted for a given material velocity, the delay control should be adjusted until a correct thickness reading is obtained on the instrument. However, if the instrument must be completely standardized with the delay line search unit, the following technique is recommended:

**8.2.2.1** Use at least two standardization blocks. One should have a thickness near the maximum of the range to be measured and the other block near the minimum thickness. For convenience, it is desirable that the thickness should be “round numbers” so that the difference between them also has a convenient “round number” value.

**8.2.2.2** Place the search unit sequentially on one and then the other block, and obtain both readings. The difference between these two readings should be calculated. If the reading thickness difference is less than the actual thickness difference, place the search unit on the thicker specimen, and adjust the material standardize control to expand the thickness range. If the reading thickness difference is greater than the actual thickness difference, place the search unit on the thicker specimen, and adjust the material standardize control to decrease the thickness range. A certain amount of over correction