



Designation: D7070 – 16

Standard Test Methods for Creep of Rock Core Under Constant Stress and Temperature¹

This standard is issued under the fixed designation D7070; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope*

1.1 These test methods cover the creep behavior of intact weak and hard rock core in fixed states of stress at ambient (room) or elevated temperatures. For creep behavior at lower temperatures refer to Test Method [D5520](#). The methods specify the apparatus, instrumentation, and procedures necessary to determine the strain as a function of time under sustained load at constant temperature and when applicable, constant humidity.

1.1.1 Hard rocks are considered those with a maximum axial strain at failure of less than 2 %. Weak rocks include such materials as salt, potash, shale, and weathered rock, which often exhibit very large strain at failure.

1.2 This standard consists of three methods that cover the creep capacity of core specimens.

1.2.1 *Method A*—Creep of Hard Rock Core Specimens in Uniaxial Compression at Ambient or Elevated Temperature.

1.2.2 *Method B*—Creep of Weak Rock Core Specimens in Uniaxial Compression at Ambient or Elevated Temperature.

1.2.3 *Method C*—Creep of Rock Core Specimens in Triaxial Compression at Ambient or Elevated Temperature.

1.3 All observed and calculated values shall conform to the guidelines for significant digits and rounding established in Practice [D6026](#).

1.4 The procedures used to specify how data are collected/recorded and calculated in this standard are regarded as the industry standard. In addition, they are representative of the significant digits that generally should be retained. The procedures used do not consider material variation, purpose for obtaining data, special purpose studies, or any considerations for the user's objectives; and it is common practice to increase or reduce significant digits of reported data to commensurate with these considerations. It is beyond the scope of these test methods to consider significant digits used in analysis methods for engineering design.

1.5 *Units*—The values stated in SI units are to be regarded as the standard. The values given in parentheses are mathematical conversions to inch-pound units that are provided for information only and are not considered standard.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and to determine the applicability of regulatory limitations prior to use. For specific precautionary statements, see Section 7.*

2. Referenced Documents

2.1 ASTM Standards:²

- [D653 Terminology Relating to Soil, Rock, and Contained Fluids](#)
- [D2113 Practice for Rock Core Drilling and Sampling of Rock for Site Exploration](#)
- [D2216 Test Methods for Laboratory Determination of Water \(Moisture\) Content of Soil and Rock by Mass](#)
- [D2845 Test Method for Laboratory Determination of Pulse Velocities and Ultrasonic Elastic Constants of Rock](#)
- [D3740 Practice for Minimum Requirements for Agencies Engaged in Testing and/or Inspection of Soil and Rock as Used in Engineering Design and Construction](#)
- [D4543 Practices for Preparing Rock Core as Cylindrical Test Specimens and Verifying Conformance to Dimensional and Shape Tolerances](#)
- [D5079 Practices for Preserving and Transporting Rock Core Samples](#)
- [D5520 Test Method for Laboratory Determination of Creep Properties of Frozen Soil Samples by Uniaxial Compression](#)
- [D6026 Practice for Using Significant Digits in Geotechnical Data](#)
- [E4 Practices for Force Verification of Testing Machines](#)
- [E122 Practice for Calculating Sample Size to Estimate, With Specified Precision, the Average for a Characteristic of a Lot or Process](#)

¹ This test method is under the jurisdiction of ASTM Committee [D18](#) and is the direct responsibility of Subcommittee [D18.12](#) on Rock Mechanics.

Current edition approved Nov. 1, 2016. Published November 2016. Originally approved in 2004. Last previous edition approved in 2008 as D7070 - 08. DOI: 10.1520/D7070-16.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

*A Summary of Changes section appears at the end of this standard

3. Terminology

3.1 Definitions:

3.1.1 For definitions of common technical terms used in this standard, refer to Terminology **D653**.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *hard rock*—rock core exhibiting less than 2 % strain at failure when tested in uniaxial compression.

3.2.2 *weak rock*—rock core exhibiting 2 % or greater strain at failure when tested in uniaxial compression.

3.2.3 *true stress*—a constant stress applied to a specimen as a result of a varying vertical load based upon changes in the specimen diameter.

4. Summary of Test Method

4.1 A section of rock core is cut to length, and the ends are machined flat or are capped in a manner to produce a cylindrical test specimen.

4.2 For Methods A and B, (Uniaxial Compression Method) the specimen is positioned onto a loading frame. A specified axial load is applied rapidly to the specimen and sustained throughout the test duration. The specimen may be subjected to an elevated temperature and/or constant humidity environment if so desired. The axial deformation is monitored as a function of elapsed time. The lateral deformation may also be monitored as a function of elapsed time if so desired.

4.3 For Method C (Triaxial Compression Method), the specimen is placed into a triaxial chamber and then positioned onto a loading frame. The specimen is subjected to a constant confining pressure. A specified axial load is rapidly applied to the specimen and maintained throughout the test duration. If desired, the specimen, while positioned in the triaxial cell, can be subjected to elevated temperature. The axial deformation is monitored as a function of elapsed time. The lateral deformation may also be monitored as a function of elapsed time if so desired.

5. Significance and Use

5.1 There are many underground structures that are constructed for permanent or long-term use. Often, these structures are subjected to a relatively constant load. Creep tests provide quantitative parameters for stability analysis of these structures.

5.2 The deformation and strength properties of rock cores measured in the laboratory usually do not accurately reflect large-scale in situ properties, because the latter are strongly influenced by joints, faults, inhomogeneities, weakness planes, and other factors. Therefore, laboratory test results of intact specimens shall be utilized with proper judgment in engineering applications.

NOTE 1—The statements on precision and bias contained in this test method; the precision of this test method is dependent on the competence of the personnel performing it, and the suitability of the equipment and facilities used. Agencies that meet the criteria of Practice **D3740** are generally considered capable of competent and objective testing. Users of this test method are cautioned that compliance with Practice **D3740** does not in itself assure reliable testing. Reliable testing depends on many

factors; Practice **D3740** provides a means of evaluating some of these factors.

6. Apparatus

6.1 *Loading Device*—The loading device shall be of sufficient capacity to meet the requirements of the testing program and capable of applying the test load at a rate conforming to the requirements specified in **9.5**. The device shall be capable of maintaining the specified test load to within $\pm 2\%$. The force measurement device or load cell shall be calibrated in accordance with the procedures outlined in Practice **E4** and following the schedule provided in Practice **D3740**.

NOTE 2—By definition, creep is the time-dependent deformation under constant stress. The loading device is specified to maintain constant axial load and therefore, constant engineering stress. The true stress, however, decreases as the specimen deforms and the cross-sectional area increases. Because of the associated experimental ease, constant load testing is recommended. However, the procedure permits constant true-stress testing, provided that the applied load is increased with specimen deformation so that true stress is constant within $\pm 2\%$.

6.2 *Triaxial Apparatus*—The triaxial apparatus shall consist of a chamber in which the test specimen is subjected to a constant lateral hydraulic pressure and the required axial load. The triaxial apparatus shall have a working pressure that exceeds the specified confining stress. The triaxial apparatus shall have safety valves where applicable, suitable entry ports for filling the chamber, hoses, pressure gauges, and shutoff valves as required. **Fig. 1** shows a typical test apparatus and associated equipment.

6.3 *Triaxial Flexible Membrane*—The membrane encases the rock specimen and extends over the platens to prevent infiltration of the confining fluid. A sleeve of natural or synthetic rubber or plastic is satisfactory for ambient (room) temperature tests. Metal or high-temperature rubber jackets such as viton are normally required for elevated temperature tests. The membrane shall be inert relative to the confining fluid and shall cover small pores in the sample without rupturing when the confining pressure is applied. Plastic or silicone rubber coatings may be applied directly to the sample, provided these materials do not penetrate or strengthen the specimen. Care must be exercised to form an effective seal where the platen and specimen meet. Membranes formed by coatings shall be subject to the same performance requirements as elastic sleeve membranes.

6.4 *Triaxial Pressure-Maintaining Device*—A hydraulic pump, pressure intensifier, or other system of sufficient capacity to maintain constant the desired lateral pressure. The pressurization system shall be capable of maintaining the confining pressure constant to within $\pm 1\%$ throughout the test duration. The confining pressure shall be measured with a hydraulic pressure gauge or electronic transducer and readout having an accuracy of at least $\pm 1\%$ of the confining pressure and a resolution of at least 0.5 % of the confining pressure.

6.5 *Confining-Pressure Fluids*—For ambient (room) temperature tests, hydraulic fluids compatible with the pressure-maintaining device shall be used. For elevated temperature tests the fluid shall remain stable at the temperature and pressure levels designated for the test.

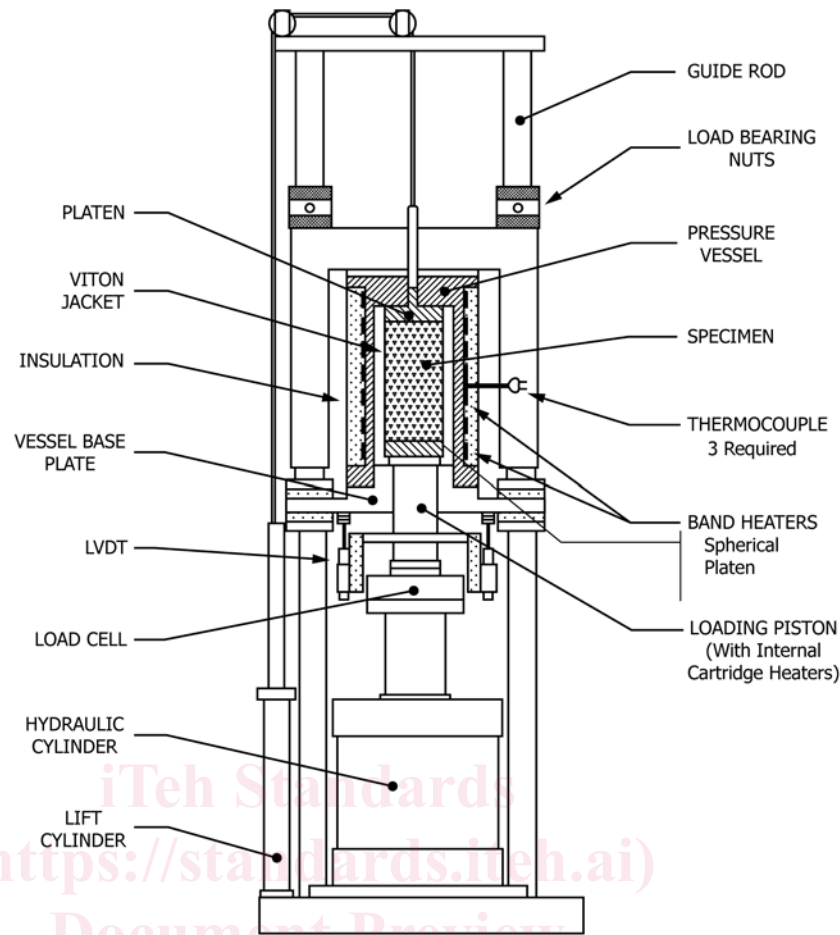


FIG. 1 Typical Triaxial Test Apparatus

6.6 *Elevated-Temperature Device*—The elevated temperature device may be an enclosure that fits in or over the loading apparatus, for Method A and B tests. For Method C (triaxial) tests an internal system that fits in the triaxial apparatus, an external system encompassing the triaxial cell or an enclosure that completely encompasses the entire test apparatus may be used. The enclosure, used for Methods A and B, may be equipped with humidity control for testing specimens in which the moisture content is to be controlled.

6.6.1 For high temperatures, a system of heaters, insulation, and temperature measuring devices are normally required to maintain the specified temperature. Temperature shall be measured at three locations, with one sensor positioned near the top, one at midheight, and one near the bottom of the specimen. The average specimen temperature shall be maintained to within $\pm 1^\circ\text{C}$ ($\pm 2^\circ\text{F}$) of the required test temperature and be based solely on the midheight sensor readings. The maximum temperature difference between the midheight sensor and either end sensor shall not exceed $\pm 3^\circ\text{C}$ ($\pm 5^\circ\text{F}$).

6.6.2 An alternative to measuring the temperature at three locations along the specimen during the test is to determine the temperature distribution in a substitute specimen that has temperature sensors located in ports at three positions similar to the configuration of the actual test specimen and having the same temperature requirements as outlined in 6.6.1.

6.6.3 The enclosure shall be equipped with humidity control for testing specimens in which the moisture content is to be kept constant. A controlled humidity enclosure shall be used when testing weak rock such as shale or weathered rock that may be susceptible to cracking or degrading due to moisture loss. In place of a humidity enclosure, the test load apparatus may be housed in a humidity controlled room.

6.7 *Temperature Measuring Device*—Thermocouples or platinum resistance thermometers (RTDs) having an accuracy of $\pm 1^\circ\text{C}$ ($\pm 2^\circ\text{F}$) with a resolution of 0.1°C (0.2°F).

6.8 *Platens*—Two steel platens are used to transmit the axial load to the ends of the specimen. They shall have a hardness of 58 HRC or greater. One of the platens shall be spherically seated and the other a plain rigid platen. The bearing faces shall not depart from a plane by more than 0.015 mm (0.0006 in.) when the platens are new and shall be maintained within a permissible variation of 0.025 mm (0.0010 in.). The diameter of the spherical seat shall be at least as large as that of the test specimen but shall not exceed twice the diameter of the test specimen. The center of the sphere in the spherical seat shall coincide with that of the bearing face of the specimen. The spherical seat shall be properly lubricated to ensure free movement. The movable portion of the platen shall be held