



Standard Test Methods for Sheathed Thermocouples and Sheathed Thermocouple Cable¹

This standard is issued under the fixed designation E839; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

^{ε1} NOTE—Added references to Tables X1.7 and X1.8 to 10.7.4 editorially in December 2016.

1. Scope

1.1 This document lists methods for testing Mineral-Insulated, Metal-Sheathed (MIMS) thermocouple assemblies and thermocouple cable, but does not require that any of these tests be performed nor does it state criteria for acceptance. The acceptance criteria are given in other ASTM standard specifications that impose this testing for those thermocouples and cable. Examples from ASTM thermocouple specifications for acceptance criteria are given for many of the tests. These tabulated values are not necessarily those that would be required to meet these tests, but are included as examples only.

1.2 These tests are intended to support quality control and to evaluate the suitability of sheathed thermocouple cable or assemblies for specific applications. Some alternative test methods to obtain the same information are given, since in a given situation, an alternative test method may be more practical. Service conditions are widely variable, so it is unlikely that all the tests described will be appropriate for a given thermocouple application. A brief statement is made following each test description to indicate when it might be used.

1.3 The tests described herein include test methods to measure the following properties of sheathed thermocouple material and assemblies.

1.3.1 Insulation Properties:

1.3.1.1 *Compaction*—direct method, absorption method, and tension method.

1.3.1.2 Thickness.

1.3.1.3 *Resistance*—at room temperature and at elevated temperature.

1.3.2 Sheath Properties:

1.3.2.1 *Integrity*—two water test methods and mass spectrometer.

1.3.2.2 *Dimensions*—length, diameter, and roundness.

1.3.2.3 *Wall thickness.*

1.3.2.4 *Surface*—gross visual, finish, defect detection by dye penetrant, and cold-lap detection by tension test.

1.3.2.5 *Metallurgical structure.*

1.3.2.6 *Ductility*—bend test and tension test.

1.3.3 Thermoelement Properties:

1.3.3.1 *Calibration.*

1.3.3.2 *Homogeneity.*

1.3.3.3 *Drift.*

1.3.3.4 *Thermoelement diameter, roundness, and surface appearance.*

1.3.3.5 *Thermoelement spacing.*

1.3.3.6 *Thermoelement ductility.*

1.3.3.7 *Metallurgical structure.*

1.3.4 Thermocouple Assembly Properties:

1.3.4.1 *Dimensions*—length, diameter, and roundness.

1.3.4.2 *Surface*—gross visual, finish, reference junction end moisture seal, and defect detection by dye penetrant.

1.3.4.3 *Electrical*—continuity, loop resistance, and connector polarity.

1.3.4.4 *Radiographic inspection.*

1.3.4.5 *Thermoelement diameter.*

1.3.4.6 *Thermal response time.*

1.3.4.7 *Thermal cycle.*

1.4 The values stated in either SI units or inch-pound units are to be regarded separately as standard. The values stated in each system may not be exact equivalents; therefore, each system shall be used independently of the other. Combining values from the two systems may result in non-conformance with the standard.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

1.6 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the*

¹ These test methods are under the jurisdiction of ASTM Committee E20 on Temperature Measurement and is the direct responsibility of Subcommittee E20.14 on Thermocouples - Testing.

Current edition approved Nov. 1, 2011. Published January 2016. Originally approved in 1989. Last previous edition approved in 2011 as E839 – 11. DOI: 10.1520/E0839-11R16E01.

Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.

2. Referenced Documents

2.1 ASTM Standards:²

- E3 Guide for Preparation of Metallographic Specimens
- E94 Guide for Radiographic Examination Using Industrial Radiographic Film
- E112 Test Methods for Determining Average Grain Size
- E165 Practice for Liquid Penetrant Testing for General Industry
- E177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods
- E207 Test Method for Thermal EMF Test of Single Thermoelement Materials by Comparison with a Reference Thermoelement of Similar EMF-Temperature Properties
- E220 Test Method for Calibration of Thermocouples By Comparison Techniques
- E230 Specification for Temperature-Electromotive Force (emf) Tables for Standardized Thermocouples
- E235 Specification for Type K and Type N Mineral-Insulated, Metal-Sheathed Thermocouples for Nuclear or for Other High-Reliability Applications
- E344 Terminology Relating to Thermometry and Hydrometry
- E585/E585M Specification for Compacted Mineral-Insulated, Metal-Sheathed, Base Metal Thermocouple Cable
- E608/E608M Specification for Mineral-Insulated, Metal-Sheathed Base Metal Thermocouples
- E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method
- E780 Test Method for Measuring the Insulation Resistance of Mineral-Insulated, Metal-Sheathed Thermocouples and Mineral-Insulated, Metal-Sheathed Cable at Room Temperature
- E1025 Practice for Design, Manufacture, and Material Grouping Classification of Hole-Type Image Quality Indicators (IQI) Used for Radiography
- E1129/E1129M Specification for Thermocouple Connectors
- E1350 Guide for Testing Sheathed Thermocouples, Thermocouple Assemblies, and Connecting Wires Prior to, and After Installation or Service
- E1684 Specification for Miniature Thermocouple Connectors
- E1751 Guide for Temperature Electromotive Force (emf) Tables for Non-Letter Designated Thermocouple Combinations
- E2181/E2181M Specification for Compacted Mineral-Insulated, Metal-Sheathed, Noble Metal Thermocouples and Thermocouple Cable

2.2 ANSI Standard

B 46.1 Surface Texture³

2.3 Other Standard

USAEC Division of Reactor Development and Technology
RDT Standard C 2-1T Determination of Insulation Compaction in Ceramic Insulated Conductors August 1970

3. Terminology

3.1 *Definitions*—The definitions given in Terminology E344 shall apply to these test methods.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *bulk cable, n*—a single length of thermocouple cable produced from the same raw material lots after completion of fabrication.

3.2.2 *cable lot, n*—a quantity of finished mineral-insulated, metal-sheathed thermocouple cable manufactured from tubing or other sheath material from the same heat, wire from the same spool and heat, and insulation from the same batch, then assembled and processed together under controlled production conditions to the required final outside diameter.

3.2.3 *cold-lap, n*—sheath surface defect where the sheath surface has been galled and torn by a drawing die and the torn surface smoothed by a subsequent diameter reduction.

3.2.4 *insulation compaction density, n*—the density of a compacted powder is the combined density of the powder particles and the voids remaining after the powder compaction. Sometimes the insulation compaction density is divided by the theoretical density of the powder particles to obtain a dimensionless fraction of theoretical density as a convenient method to express the relative compaction.

3.2.5 *raw material, n*—tubing or other sheath material, insulation and wires used in the fabrication of sheathed thermocouple cable.

3.2.6 *short range ordering, n*—the reversible short-ranged, order-disorder transformation in which the nickel and chromium atoms occupy specific (ordered) localized sites in the Type EP or Type KP thermoelement alloy crystal structure.

3.2.7 *thermal response time, n*—the time required for a sheathed thermocouple signal to attain the specified percent of the total voltage change produced by a step change of temperature at the sheath's outer surface.

4. Summary of Test Methods

4.1 Insulation Properties:

4.1.1 *Compaction*—These tests ensure that the insulation is compacted sufficiently (1) to prevent the insulation from shifting during use with the possibility of the thermoelements shorting to each other or to the sheath, and (2) to have good heat transfer between the sheath and the thermoelements.

4.1.2 *Insulation Resistance*—The insulation shall be free of moisture and contaminants that would compromise the voltage-temperature relationship or shorten the useful life of

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036.

the sheathed thermocouple. Measurement of insulation resistance is a useful way to detect the presence of unacceptable levels of impurities in the insulation.

4.2 *Sheath Properties:*

4.2.1 *Integrity*—These tests ensure that (1) the sheath will be impervious to moisture and gases so the insulation and thermoelements will be protected, (2) surface flaws and cracks that might develop into sheath leaks are detected, and (3) the sheath walls are as thick as specified.

4.2.2 *Dimensions*—Determination of length, diameter, and sheath roundness are often necessary to assure proper dimensional fit.

4.2.3 *Sheath Ductility*—The sheath shall be ductile enough to bend the required amount without breaking or cracking.

4.3 *Thermoelement Properties Service Life:*

4.3.1 *Calibration*—This test ensures that the temperature-emf relationship initially corresponds to standardized tolerances.

4.3.2 *Size*—The thermocouple sheath and thermoelement sizes are related to the service life and the thermoelement spacing is related to possible low insulation resistance or shorting.

4.3.3 *Thermoelement Ductility*—Ductility of the thermoelements shall be sufficient to allow the assembly to be bent during assembly or service without significant damage to the thermoelements.

4.4 *Thermocouple Assembly Properties*—The criteria listed above shall apply to both thermocouple assemblies and to bulk cable. In addition, the following tests are important for thermocouple assemblies.

4.4.1 *Continuity*—The loop continuity test assures that the thermocouple assembly has a completed circuit.

4.4.2 *Loop Resistance*—The loop resistance test can detect shorted or damaged thermoelements.

4.4.3 *Polarity*—The connector polarity test indicates whether the connector is correctly installed.

4.4.4 *Moisture Seal*—The moisture seal at the reference junction end of the thermocouple, if faulty, may allow contamination of the insulation with moisture or gases.

4.4.5 *Radiography*—Radiographic examination of the junction and sheath closure weld can indicate faulty junctions and sheath closures that will lead to early failure. Most internal dimensions can also be measured from the radiograph.

4.4.6 *Response Time*—The thermal response time gives an indication of the quickness with which an installed thermocouple will signal a changing temperature under the test conditions.

4.4.7 *Thermal Cycle*—The thermal cycle test will offer assurance that the thermocouple will not have early failure because of strains imposed from temperature transients.

5. Significance and Use

5.1 This standard provides a description of test methods used in other ASTM specifications to establish certain acceptable limits for characteristics of thermocouple assemblies and thermocouple cable. These test methods define how those characteristics shall be determined.

5.2 The usefulness and purpose of the included tests are given for the category of tests.

5.3 **Warning**—Users should be aware that certain characteristics of thermocouples might change with time and use. If a thermocouple's designed shipping, storage, installation, or operating temperature has been exceeded, that thermocouple's moisture seal may have been compromised and may no longer adequately prevent the deleterious intrusion of water vapor. Consequently, the thermocouple's condition established by test at the time of manufacture may not apply later. In addition, inhomogeneities can develop in thermoelements because of exposure to higher temperatures, even in cases where maximum exposure temperatures have been lower than the suggested upper use temperature limits specified in Table 1 of Specification E608/E608M. For this reason, calibration of thermocouples destined for delivery to a customer is not recommended. Because the EMF indication of any thermocouple depends upon the condition of the thermoelements along their entire length, as well as the temperature profile pattern in the region of any inhomogeneity, the EMF output of a used thermocouple will be unique to its installation. Because temperature profiles in calibration equipment are unlikely to duplicate those of the installation, removal of a used thermocouple to a separate apparatus for calibration is not recommended. Instead, *in situ* calibration by comparison to a similar thermocouple known to be good is often recommended.

6. General Requirements

6.1 All the inspection operations are to be performed under clean conditions that will not degrade the insulation, sheath, or thermoelements. This includes the use of suitable gloves when appropriate.

6.2 During all process steps in which insulation is exposed to ambient atmosphere, the air shall be clean, with less than 50 % relative humidity, and at a temperature between 20 and 26°C (68 and 79°F).

6.3 All samples which are tested shall be identified by material code, and shall be traceable to a production run.

7. Insulation Properties

7.1 *Insulation Compaction Density*—The thermal conductivity of the insulation, as well as the ability of the insulation to lock the thermoelements into place, will be affected by the insulation compaction density.

7.1.1 A direct method for measuring insulation compaction density is applicable if a representative sample can be sectioned so that the sample ends are perpendicular to the sample length and the sheath, thermoelements, and insulation form a smooth surface free of burrs. The procedure is as follows:

7.1.1.1 Weigh the sample section,

7.1.1.2 Measure the sheath diameter and length with a micrometer,

7.1.1.3 Separate the insulation from the thermoelement and sheath with the use of an air abrasive tool,

7.1.1.4 Weigh the thermoelements and sheath, and

7.1.1.5 Determine the sheath and thermoelements densities either by experiment or from references.

7.1.1.6 Determine the percentage of the maximum theoretical insulation density ρ as follows:

$$\% \rho = 100(A - B) / \{ [0.785 C^2 D - (E/F + G/H)] J \} \quad (1)$$

where:

- A = total specimen mass, kg or lb,
- B = sheath and wires mass, kg or lb,
- C = sheath diameter, m or in.,
- D = specimen length, m or in.,
- E = sheath mass, kg or lb,
- F = sheath density, kg/m³ or lb/in.³,
- G = wires mass, kg or lb,
- H = wires density (averaged density if applicable), kg/m³ or lb/in.³, and
- J = maximum theoretical density of the insulation, kg/m³ or lb/in.³.

7.1.2 Alternately, a liquid absorption method for determining the insulation compaction density may be utilized for MIMS samples with outside diameters 1.5 mm (.062 in.) and larger. This method is based upon a procedure detailed in RDT C 2-1T and requires the following: (1) the sample ends shall be perpendicular to the sample axis and have a smooth, unglazed surface which will readily absorb liquid and shall be free of burrs, (2) the outer surfaces of the thermoelements and the inner surface of the sheath shall be smooth and non-absorbent, and (3) the insulation shall readily support capillary absorption through the entire length of the sample. This procedure is as follows:

7.1.2.1 Determine the density of kerosene for the temperature at which the measurement is being performed if other than 16°C (60°F).

7.1.2.2 Cut a specimen approximately 2.5 mm (1 in.) long.

7.1.2.3 Measure and record the inside diameter of the cable's sheath and the outside diameter of the cable's thermoelements to within .025 mm (.001 in.).

7.1.2.4 Weigh the specimen and record its weight.

7.1.2.5 Measure and record the specimen's length to within .025 mm (.001 in.) using a vernier caliper.

7.1.2.6 Immerse the specimen in kerosene for a minimum of 24 h.

7.1.2.7 Re-weigh the specimen and record its weight.

7.1.2.8 Determine the percentage of the maximum theoretical insulation density ρ as follows:

$$\% \rho = 100 [1 - \{ (Y - X) / 0.785 S L \{ O^2 - PR^2 \} \}] \quad (2)$$

- L = specimen length, cm or in.,
- O = inside diameter of sheath, cm or in.,
- P = number of thermoelements in the cable,
- R = outside diameter of thermoelements, cm or in.,
- S = specific gravity of the kerosene absorbed at 16°C (60°F), .81715 g/cm³ or .02952 lb/in.³,
- X = weight of the specimen before kerosene is absorbed, g or lb, and
- Y = weight of the specimen after kerosene is absorbed, g or lb.

7.2 *Insulation Compaction, Assurance Test*—This is a destructive test on representative samples that determines if the thermoelements are locked together with the sheath by the compacted insulation, but this test does not measure the

compaction density per se. This test is the complement of the tests of 7.1 and 7.2 that measures the insulation compaction density but does not establish that the thermoelements are locked to the sheath, since there is no established minimum compaction density where locking begins. This test can be performed concurrently with the tension test in 8.5.3.

7.2.1 Cut a test specimen about 0.5 m (20 in.) long from one end of a bulk cable length and strip both ends of the specimen to expose a minimum of 10 mm (0.4 in.) of the thermoelements.

7.2.2 Without sealing the exposed insulation, clean the thermoelements of insulation to provide good electrical contact and twist the wires together on one end to form a thermocouple loop (see Fig. 1).

7.2.3 Measure the electrical resistance of the thermocouple loop to $\pm 0.01 \Omega$ and measure the length of the thermocouple loop to establish the electrical resistance per unit length.

7.2.4 Place the test sample in the tension testing machine so that (1) the grips clamp only on the sample sheath, (2) the force will be applied longitudinally on the sheath, and (3) there is at least a 0.25-m (10-in.) distance between the grips where the force will be applied (see Fig. 2).

7.2.5 Attach an ohmmeter capable of measuring $\pm 0.01 \Omega$ to the exposed thermoelements and measure the resistance with no tension force applied; also measure the distance between the tension tester grips to establish the initial length, L_0 , of the test sample that will be elongated.

7.2.6 Calculate the initial resistance, R_0 , of the test specimen section that will be elongated, using the unit length electrical resistance obtained in 7.2.3.

7.2.7 Make a simultaneous record of the electrical resistance and the elongation of the sheath while stretching the test sample until the thermoelements break.

7.2.8 Examine the exposed ends of the thermoelements to see whether they have been drawn into the insulation during the elongation; any shortening of the exposed ends indicates low compaction of the insulation.

7.2.9 Plot the fractional change of resistance ($\Delta R/R_0$) versus the fractional change of length ($\Delta L/L_0$). The slope of the plot reveals if the thermoelements were locked to the sheath throughout the plastic deformation of the sheath and, if not, where the thermoelements began to elongate in a different manner than the sheath. Examples of criteria to evaluate the insulation locking are given in X1.9

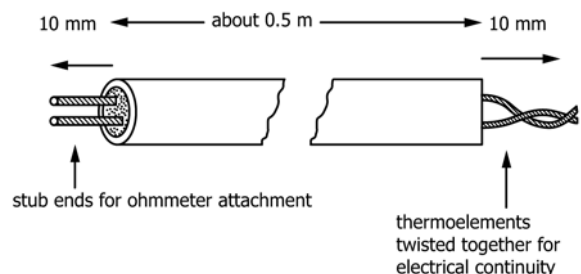


FIG. 1 Specimen of Sheathed Thermocouple Cable Prepared for Tension Testing

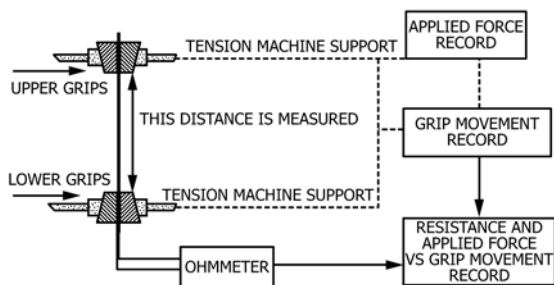


FIG. 2 The Thermocouple Positioned in the Tension Tester

7.3 *Insulation Thickness Measurement*—Determine the insulation thickness, dimension *C* of Fig. 3, using either of the following methods:

7.3.1 A metallographic mount, prepared in accordance with Practice E3, of a polished cross section of the thermocouple or cable using a microscope having at least a 60× magnification and a 2.5-mm (0.1-in.) reticle graduated in at least 0.03-mm (0.001-in.) increments. This measurement test can be done at the same time as the measurements in 8.2.4.1 and 9.4.2.

7.3.2 A radiograph, or a projected enlargement of the radiograph, can be used with the microscope described in 7.3.1 to measure the insulation thickness *C* of Fig. 3 around the measuring junction. See also 10.7, Radiographic Inspection.

7.3.3 Sampling frequency, measurement tolerance, and insulation thickness shall be as stated in the standard specification relevant to the subject thermocouple. Examples of specifications for the insulation thickness are given in the Measuring Junction Configuration section of Specifications E608/E608M and E2181/E2181M for the junction area, in the General Dimensional Requirements of Specifications E585/E585M and E2181/E2181M and in Tables X1.1 and X1.2.

7.4 *Insulation Resistance, Room Temperature*—Measure the insulation resistance of sheathed thermocouple cable at room temperature using Test Method E780. Sampling frequency and insulation resistance shall be as stated in the relevant invoking thermocouple specification, or as agreed upon between the purchaser and the producer. See Table X1.3.

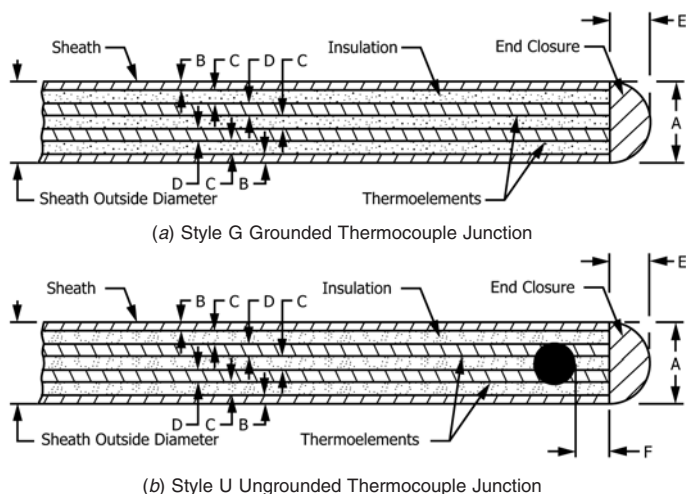


FIG. 3 Sheathed Thermocouple Assembly

7.5 *Insulation Resistance, Elevated Temperatures*—The purpose of this test is to determine if the thermocouple insulation will be adequate for high temperature use of the thermocouple (**Warning**—All thermocouples may have changes in thermoelectric homogeneity produced by exposure to elevated temperatures; therefore, this test should be regarded as usually destructive.) Sampling frequency shall be as stated in the standard specification relevant to the subject thermocouple.

7.5.1 *Thermocouple Assembly*—Measure the electrical resistance between the thermocouple circuit and the sheath of a finished thermocouple assembly with a Style U ungrounded measuring junction (see Fig. 3) using the technique of Test Method E780. Insert the measuring junction of the finished thermocouple into a furnace or constant temperature bath to a depth that will yield maximum temperature stability (example: 20 sheath diameters). Then, the thermocouple junction can be heated to the test temperature. This procedure is not applicable to a Style G grounded measuring junction thermocouple assembly.

7.5.1.1 The minimum acceptable insulation resistance between the thermoelements and the sheath while the test specimen is at the specified elevated temperature shall be as stated in the standard specification relevant to the subject thermocouple assembly.

7.5.2 *Bulk Cable*—Insulation resistance tests on sheathed thermocouple cable at elevated temperatures have the purpose of determining (1) if excess moisture is in the insulation of the bulk cable, or (2) if the insulation contains excess impurities other than moisture, which will affect the insulation resistance at high temperatures.


7.5.2.1 *Elevated Temperature, Moisture and Impurities Combined*—The steps listed for this test are intended to evaluate the combined effects of insulation impurities and moisture contamination using elevated temperature insulation resistance testing of Type K or N bulk cable. **Warning**—Improper technique in constructing thermocouple assemblies can introduce additional insulation impurities and moisture contamination.

(1) Cut a specimen of approximately 1.2 m (4 ft) in length from the end of the bulk cable. Strip both ends of the sample about 25 mm (1 in.) to expose the thermoelements and at once seal the ends with an insulating sealant such as epoxy to prevent further moisture absorption. Wind the center section of the specimen around a 25-mm (1-in.) mandrel to form three coils, as shown in Fig. 4. The coils use about 0.3 m (1 ft) of the specimen.

(2) Install a suitable connector on one end of the coil and test the room temperature insulation resistance as described in 7.4.

(3) Insert the sample coil into a furnace and bring the coil temperature to $1000 \pm 10^\circ\text{C}$ ($1832 \pm 18^\circ\text{F}$). The sealed ends of the sample should be kept near room temperature. Allow the sample to stabilize at 1000°C (1832°F) as measured by the furnace monitor thermocouple for at least 15 min.

(4) Measure the insulation resistance at the voltage and range appropriate for readability and the thermocouple sheath diameter. The charge time of the megohm tester should be at least 1 min before the measurement is recorded.

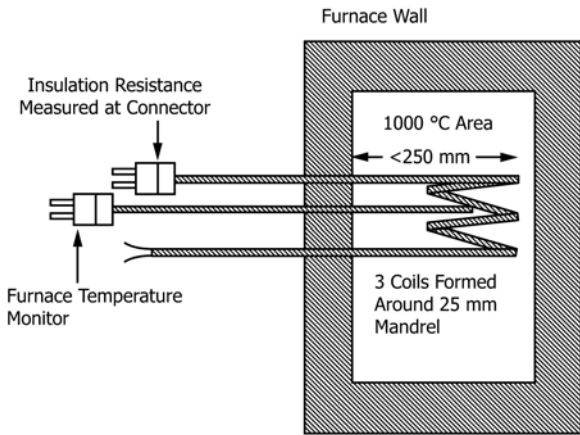

NOTE 1—The ends of the test specimen are sealed with epoxy to prevent water vapor from being adsorbed or desorbed during the test.

FIG. 4 High Temperature Insulation Resistance Test Assembly to Test for Moisture Plus Impurities


(5) Record the insulation resistance between each thermoelement, and from each thermoelement to the sheath.

7.5.2.2 *Elevated Temperature, Contaminants Other than Moisture*—The steps listed for this test evaluate the effects of impurities other than moisture in the insulation using insulation resistance testing of the bulk cable at elevated temperatures.

(1) Cut a specimen about 0.6 m (2 ft) long from the end of the bulk cable to be tested. Strip both ends about 25 mm (1 in.) to expose the thermoelements.

(2) Weld extension wires to each of the thermoelements and to the sheath, as shown in Fig. 5. The extension wires need not be the same composition as the thermoelements, but the extension wire must withstand the temperature of the test and the same composition extension wire should be used for all connections to the specimen.

(3) Wind the center section of the specimen around a 25-mm (1-in.) mandrel to form three coils, as shown in Fig. 5. The coils use about 0.3 m (1 ft) of the sample.

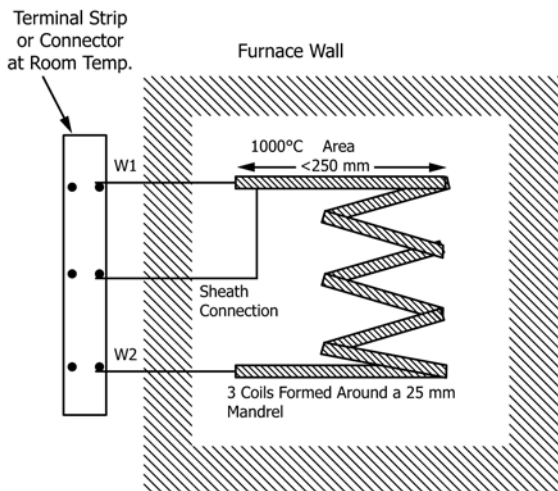

NOTE 1—The ends of the test specimen are not sealed, allowing water vapor to escape before measuring the insulation resistance

FIG. 5 High Temperature Insulation Resistance Test, Insulation Contamination Other Than Moisture

(4) Install a suitable terminal strip or connector to the extension wires, as shown in Fig. 5 and test the room temperature insulation resistance as described in 7.4.

(5) Insert the sample coil into a furnace so that the extension wires are in the same uniform temperature zone as the coil and bring the coil temperature to $1000 \pm 10^\circ\text{C}$ ($1832 \pm 18^\circ\text{F}$). Allow the sample to stabilize at the test temperature as measured by the furnace monitor thermocouple for at least 15 min.

(6) Measure the insulation resistance at the voltage appropriate for the thermocouple sheath diameter. The charge time of the megohm tester should be at least 1 min before the measurement is recorded.

(7) Record the resistance between each thermoelement, and from each thermoelement to the sheath.

8. Sheath Properties

8.1 *Sheath Integrity*—Leakage of air or moisture into the sheath can be detrimental to the life and local homogeneity of the sheathed thermoelements. Penetrations of the sheath may be caused by holes left during the fabrication of the sheath tubing, cracks due to welding, holes because of incomplete closures at either of the measurement ends, or other mechanical damage. Two major methods, water penetration and mass spectrometer measurements of helium penetration, are commonly used to assess sheath integrity. The mass spectrometer method is the most sensitive and the only one that can be used with Style G grounded measuring junction thermocouples. These sheath integrity test methods are given in order of increasing test sensitivity and difficulty. Before any sheath integrity tests are performed, wipe the sheath with a rag dampened in solvent, such as alcohol, to remove oily surface contaminants.

8.1.1 *Fast Sheath Integrity Test Using Water*—This test is usually performed on bulk cable using a less sensitive ohmmeter and a lower voltage test than the test used in 8.1.2; it is the fastest test, intended to detect the larger sheath penetrations.

8.1.1.1 Strip one end of the length of sheathed cable to expose at least 6 mm (0.25 in.) of thermoelements.

8.1.1.2 Check the opposite end of the length for any evidence of shorting of thermoelements to the sheath.

8.1.1.3 Seal the exposed ends of the compacted oxide insulation with an insulating sealant to prevent the absorption of water vapor.

8.1.1.4 Using a direct-current (dc) ohmmeter, reading to at least 20 megohm, connect the ground lead to the cable sheath and the other test lead to either thermoelement.

8.1.1.5 Then, slowly wipe the length of the sheath with a rag saturated with cold tap water. Apply a light pressure to the rag circumferentially around the sheath when wiping and start wiping from the end opposite the instrument connection.

8.1.1.6 As an alternative, immerse the entire cable length, in a coil if necessary, in tap water, except for 2 %, but not to exceed 0.3 m (1 ft), at each end.

8.1.1.7 With the ohmmeter range selection switch on the most sensitive readable range, interpret any noticeable reduction of insulation resistance as evidence of a leak in the sheath.