



# Standard Test Method for Moduli of Elasticity and Fundamental Frequencies of Carbon and Graphite Materials by Sonic Resonance<sup>1</sup>

This standard is issued under the fixed designation C747; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

<sup>ε1</sup> NOTE—Updated 9.1 and 9.2 editorially in May 2010.

## 1. Scope—Scope\*

1.1 This test method covers the measurement of the fundamental transverse, longitudinal, and torsional frequencies determination of the dynamic elastic properties of isotropic and anisotropic near isotropic carbon and graphite materials. These measured resonant frequencies are used to calculate dynamic elastic moduli for any grain orientations materials at ambient temperatures. Specimens of these materials possess specific mechanical resonant frequencies that are determined by the elastic modulus, mass, and geometry of the test specimen. The dynamic elastic properties of a material can therefore be computed if the geometry, mass, and mechanical resonant frequencies of a suitable (rectangular or cylindrical) test specimen of that material can be measured. Dynamic Young's modulus is determined using the resonant frequency in the flexural or longitudinal mode of vibration. The dynamic shear modulus, or modulus of rigidity, is found using torsional resonant vibrations. Dynamic Young's modulus and dynamic shear modulus are used to compute Poisson's ratio.

1.2 This test method determines elastic properties by measuring the fundamental resonant frequency of test specimens of suitable geometry by exciting them mechanically by a singular elastic strike with an impulse tool. Specimen supports, impulse locations, and signal pick-up points are selected to induce and measure specific modes of the transient vibrations. A transducer (for example, contact accelerometer or non-contacting microphone) senses the resulting mechanical vibrations of the specimen and transforms them into electric signals. (See Fig. 1.) The transient signals are analyzed, and the fundamental resonant frequency is isolated and measured by the signal analyzer, which provides a numerical reading that is (or is proportional to) either the frequency or the period of the specimen vibration. The appropriate fundamental resonant frequencies, dimensions, and mass of the specimen are used to calculate dynamic Young's modulus, dynamic shear modulus, and Poisson's ratio. Annex A1 contains an alternative approach using continuous excitation.

1.3 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.4 This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>2</sup>

[C215 Test Method for Fundamental Transverse, Longitudinal, and Torsional Resonant Frequencies of Concrete Specimens](#)

[C559 Test Method for Bulk Density by Physical Measurements of Manufactured Carbon and Graphite Articles](#)

[C885 Test Method for Young's Modulus of Refractory Shapes by Sonic Resonance](#)

[C1161 Test Method for Flexural Strength of Advanced Ceramics at Ambient Temperature](#)

[E111 Test Method for Young's Modulus, Tangent Modulus, and Chord Modulus](#)

[E177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods](#)

[E228 Test Method for Linear Thermal Expansion of Solid Materials With a Push-Rod Dilatometer](#)

[E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee D02 on Petroleum Products, Liquid Fuels, and Lubricants and is the direct responsibility of Subcommittee D02.F0 on Manufactured Carbon and Graphite Products.

Current edition approved May 1, 2010 Oct. 1, 2016. Published May 2010 January 2017. Originally approved in 1974. Last previous edition approved in 2005 2010 as C747-93(2005)-C747-93 (2010)<sup>ε1</sup>. DOI: 10.1520/C0747-93R10E01:10.1520/C0747-16.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For Annual Book of ASTM Standards volume information, refer to the standard's Document Summary page on the ASTM website.

\*A Summary of Changes section appears at the end of this standard

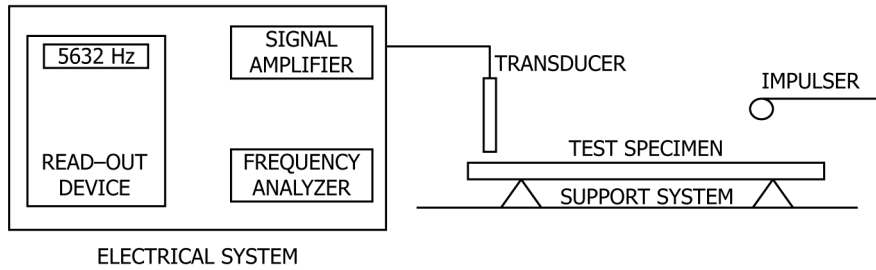


FIG. 1 - Resonance Modes Block Diagram of Typical Test Apparatus

### 3. Terminology

#### 3.1 Definitions of Terms Specific to This Standard: Definitions:

3.1.1 *antinodes, n*—two or more locations that have local maximum displacements, called antinodes, in an unconstrained slender rod or bar in resonance. For the fundamental flexure resonance, the antinodes are located at the two ends and the center of the specimen.

3.1.2 *elastic modulus*—the initial tangent modulus as defined in Test Method ratio of stress to strain, in the stress  $E_{HH}$  range where Hooke's law is valid.

3.1.3 *flexural vibrations, n*—the vibrations that occur when the displacements in a slender rod or bar are in a plane normal to the length dimension.

3.1.4 *homogeneous, adj*—in carbon and graphite technology, the condition of a specimen such that the composition and density are uniform, so that any smaller specimen taken from the original is representative of the whole. Practically, as long as the geometrical dimensions of the test specimen are large with respect to the size of individual grains, crystals, components, pores, or microcracks, the body can be considered homogeneous.

3.1.5 *in-plane flexure, n*—for rectangular parallelepiped geometries, a flexure mode in which the direction of displacement is in the major plane of the test specimen.

3.1.6 *isotropic, adj*—in carbon and graphite technology, having an isotropy ration of 0.9 to 1.1 for a specific property of interest.

3.1.7 *longitudinal vibrations*—when the oscillations in a slender rod or bar are in a plane parallel to the length dimension, the vibrations are said to be in the longitudinal mode (mode Fig. 1(a)).

3.1.8 *nodal nodes, points, n*—one or more locations in a slender rod or bar in resonance contains one or more points having zero displacement, called nodal points. In the longitudinal and torsional fundamental resonances of a uniform having a constant zero displacement. For the fundamental flexural resonance of such a rod or bar, the mid-length point is the nodal point (nodes Fig. 1(a) and Fig. 1(d)). For the fundamental transverse or flexural resonance, the nodal points are located at  $0.224 L$  from each end, where  $L$  is the length of the specimen (specimen Fig. 1(b) and Fig. 1(e)).

3.1.9 *out-of-plane flexure, n*—for rectangular parallelepiped geometries, a flexure mode in which the direction of displacement is perpendicular to the major plane of the test specimen.

3.1.10 *Poisson's ration ( $\mu$ ), n*—the absolute value of the ratio of transverse strain to the corresponding axial strain resulting from uniformly distributed axial stress below the proportional limit of the material. Young's Modulus ( $E$ ), shear modulus ( $G$ ), and Poisson's ratio ( $\mu$ ) are related by the following equation:

$$\mu = (E / 2G) - 1 \tag{1}$$

3.1.11 *resonant frequency, n*—naturally occurring frequencies of a body driven into flexural, torsional, or longitudinal vibration that are determined by the elastic modulus, mass, and dimensions of the body. The lowest resonant frequency in a given vibrational mode is the fundamental resonant frequency of that mode.

3.1.12 *shear modulus, n*—the elastic modulus in shear or torsion. Also called modulus of rigidity or torsional modulus.

3.1.13 *resonance—torsional vibrations, n*—the vibrations that occur when the oscillations in each cross-sectional plane of a slender rod or bar driven into one of the above modes of vibration is said to be in resonance when the imposed frequency is such that resultant displacements for a given amount of driving force (voltage) are at a maximum. The resonant frequency is a natural vibration frequency which is determined by the elastic moduli, density, and dimensions of the test specimen. are such that the plane twists around the length dimension axis.

3.1.5 *slender rod or bar*—a specimen whose ratio of length to minimum cross-sectional dimension is at least 5 but not more than 20.

3.1.14 *transverse vibrations—vibrations, n*—when the oscillations in a slender rod or bar are in a horizontal plane normal to the length dimension, the vibrations are said to be in the transverse mode (mode Fig. 1(b)). This mode is also commonly referred to

as the flexural mode when the oscillations are in a vertical plane (plane. Fig. 1(e)). Either the transverse or flexural mode of specimen vibration will yield the correct fundamental frequency, subject to the geometric considerations given in 9.1.

3.1.15 *torsional vibrations*—*Young's modulus, n*—when the oscillations in each cross-sectional plane of a slender rod or bar are such that the plane twists around the length dimension axis, the vibrations are said to be in the torsional mode (elastic modulus in tension or compression. Fig. 1(d)).

#### 4. Summary of Test Method

4.1 The dynamic methods of determining the elastic moduli are based on the measurement of the fundamental resonant frequencies of a slender rod of circular or rectangular cross section. The resonant frequencies are related to the specimen dimensions and material properties as follows: This test method measures the fundamental resonant frequency of test specimens of suitable geometry (bar or rod) by exciting them mechanically by a singular elastic strike with an impulse tool. A transducer (for example, contact accelerometer or non-contacting microphone) senses the resulting mechanical vibrations of the specimen and transforms them into electric signals. Specimen supports, impulse locations, and signal pick-up points are selected to induce and measure specific modes of the transient vibrations. The signals are analyzed, and the fundamental resonant frequency is isolated and measured by the signal analyzer, which provides a numerical reading that is (or is proportional to) either the frequency or the period of the specimen vibration. The appropriate fundamental resonant frequencies, dimensions, and mass of the specimen are used to calculate dynamic Young's modulus, dynamic shear modulus, and Poisson's ratio.

4.1.1 *Transverse or Flexural Mode*—The equation for the fundamental resonant frequency of the transverse or flexural mode of vibration is as follows:

$$E = CMf^2 \quad (1)$$

where:

- $E$  = elastic modulus, Pa;
- $C$  = a dimensional constant that depends upon the shape and size of the specimen, and Poisson's ratio. The units of  $C$  are to be consistent with those of  $E, M$ , and  $f$ ;
- $M$  = mass of the specimen, kg, and
- $f$  = frequency of fundamental transverse or flexural mode of vibration, Hz.

4.1.2 *Longitudinal Mode*—The equation for the fundamental resonant frequency of the longitudinal mode of variation is as follows:

$$E = Df^2 L^2 \rho \quad (2)$$

where:

- $E$  = elastic modulus, Pa;
- $D$  = a constant consistent with the units of  $E, f$ , and  $L$ ;
- $f$  = frequency of fundamental longitudinal mode of vibration, Hz;
- $L$  = length of the specimen, m, and
- $\rho$  = density of the specimen as determined by Test Method C559, kg/m<sup>3</sup>.

4.1.3 *Torsional Mode*—The equation for the fundamental resonant frequency of the torsional mode of vibration is as follows:

$$G = R B f^2 L^2 \rho \quad (3)$$

where:

- $G$  = modulus of rigidity, Pa;
- $R$  = ratio of the polar moment of inertia to the shape factor for torsional rigidity;
- $B$  = a constant consistent with the units of  $G, R, f, L$ , and  $\rho$ ;
- $f$  = frequency of fundamental torsional mode of vibration, Hz;
- $L$  = length of the specimen, m, and
- $\rho$  = density of the specimen as determined by Test Method C559, kg/m<sup>3</sup>.

#### 5. Significance and Use

5.1 This test method may be used for material development, characterization, design data generation, and quality control purposes.

5.2 This test method is primarily concerned with the room temperature determination of the dynamic moduli of elasticity and rigidity of slender rods or bars composed of homogeneously distributed carbon or graphite particles.

5.3 This test method can be adapted for other materials that are elastic in their initial stress-strain behavior, as defined in Test Method E111.

5.4 This basic test method can be modified to determine elastic moduli behavior at temperatures from  $-75^{\circ}\text{C}$  to  $+2500^{\circ}\text{C}$ .  $-75^{\circ}\text{C}$  to  $+2500^{\circ}\text{C}$ . Thin graphite rods may be used to project the specimen extremities into ambient temperature conditions to provide resonant frequency detection by the use of transducers as described in [6.4.7.1](#).

## 6. Interferences

6.1 The relationships between resonant frequency and dynamic modulus presented herein are specifically applicable to homogeneous, elastic, isotropic materials.

6.1.1 This method of determining the moduli is applicable to inhomogeneous materials only with careful consideration of the effect of inhomogeneities and anisotropy. The character (volume fraction, size, morphology, distribution, orientation, elastic properties, and interfacial bonding) of inhomogeneities in the specimens will have a direct effect on the elastic properties of the specimen as a whole. These effects must be considered in interpreting the test results for composites and inhomogeneous materials.

6.1.2 The procedure involves measuring transient elastic vibrations. Materials with very high damping capacity may be difficult to measure with this technique if the vibration damps out before the frequency counter can measure the signal (commonly within three to five cycles).

6.1.3 If specific surface treatments (coatings, machining, grinding, etching, etc.) change the elastic properties of the near-surface material, there may be accentuated effects on the properties measured by this flexural method, as compared to static bulk measurements by tensile or compression testing.

6.1.4 The test method is not satisfactory for specimens that have major discontinuities, such as large cracks (internal or surface) or voids.

6.2 This test method for determining moduli is limited to specimens with regular geometries (rectangular parallelepiped and cylinders) for which analytical equations are available to relate geometry, mass, and modulus to the resonant vibration frequencies. The test method is not appropriate for determining the elastic properties of materials that cannot be fabricated into such geometries.

6.2.1 The analytical equations assume parallel and concentric dimensions for the regular geometries of the specimen. Deviations from the specified tolerances for the dimensions of the specimens will change the resonant frequencies and introduce error into the calculations.

6.2.2 Edge treatments such as chamfers or radii are not considered in the analytical equations. Edge chamfers on flexure bars prepared according to Test Method [C1161](#) will change the resonant frequency of the test bars and introduce error into the calculations of the dynamic modulus. It is recommended that specimens for this test method not have chamfered or rounded edges.

6.2.3 For specimens with as-fabricated and rough or uneven surfaces, variations in dimensions can have a significant effect in the calculations. For example, in the calculation of dynamic modulus, the modulus value is inversely proportional to the cube of the thickness. Uniform specimen dimensions and precise measurements are essential for accurate results.

6.3 The test method assumes that the specimen is vibrating freely, with no significant restraint or impediment. Specimen supports should be designed and located properly in accordance with [9.3.1](#), [9.4.1](#), and [9.5.1](#) so the specimen can vibrate freely in the desired mode. In using direct contact transducers, the transducer should be positioned away from antinodes and with minimal force to avoid interference with free vibration. With non-contacting transducers, the maximum sensitivity is accomplished by placing the transducer at an antinode.

6.4 Proper location of the impulse point and transducer is important in introducing and measuring the desired vibration mode. The locations of the impulse point and transducer should not be changed in multiple readings; changes in position may develop and detect alternative vibration modes. In the same manner, the force used in impacting should be consistent in multiple readings.

6.5 If the frequency readings are not repeatable for a specific set of impulse and transducer locations on a specimen, it may be because several different modes of vibration are being developed and detected in the test. The geometry of the test bar and desired vibration mode should be evaluated and used to identify the nodes and antinodes of the desired vibrations. More consistent measurements may be obtained if the impulse point and transducer locations are shifted to induce and measure the single desired mode of vibration.

## 7. Apparatus

7.1 Apparatus suitable for accurately detecting, analyzing, and measuring the fundamental resonant frequency or period of a vibrating free beam is used. The test apparatus is shown in [Fig. 1](#). It consists of an impulser, a suitable pickup transducer to convert the mechanical vibration into an electrical signal, an electronic system (consisting of a signal conditioner/amplifier, a signal analyzer, and a frequency readout device), and a support system. Commercial instrumentation is available that measures the frequency or period of the vibrating specimen.

7.2 *Impulser*—The fundamental resonant frequencies for the different modes of vibration of a test specimen can be determined by several established testing procedures. The apparatus described herein uses phonograph record pickup cartridges as a convenient method of generating and detecting these frequencies. A typical testing exciting impulse is imparted by lightly striking the specimen with a suitable implement. This implement should have most of its mass concentrated at the point of impact and have mass sufficient to induce a measurable mechanical vibration, but not so large as to displace or damage the specimen physically. In practice, the size and geometry of the impulser depends on the size and weight and elastic properties of the specimen and the force



needed to produce vibration. For commonly tested geometries (small bars, rods, and discs) in advanced ceramics, an example of such an impulser would be a steel sphere 6 mm in diameter glued to the end of a flexible 10 cm long polymer rod. (See Fig. 2 apparatus is shown schematically in.) An alternative impulser would Fig. 2 be a solid metal, ceramic, or polymer sphere (2 mm to 20 mm in diameter) dropped on the specimen through a guide tube to ensure proper impulse position.

6.1.1 *Driving Circuit*—The driving circuit consists of a variable-frequency oscillator and a record pickup cartridge assembly. It is recommended that a variable-frequency oscillator be used in conjunction with a digital-frequency counter. The oscillator shall have sufficient power output to induce detectable vibrations in the test specimen at frequencies above and below the fundamental frequency under consideration. Means for controlling the output of the oscillator shall be provided. The vibrating needle of the driving unit shall be small in mass as compared to the test specimen, and a means shall be provided to maintain a minimal contact pressure on the specimen. Either a piezoelectric or magnetic driving unit meeting these requirements may be used.

6.1.2 *Pickup Circuit*—The pickup circuit consists of a record pickup cartridge, amplifier, optional high-pass filter, and an indicating meter or cathode-ray oscilloscope. The pickup unit shall generate a voltage proportional to the amplitude, velocity, or acceleration of the test specimen. Either a piezoelectric or magnetic pickup unit meeting these conditions may be used. The amplifier shall have a controllable output of sufficient magnitude to sharply peak out the resonant frequencies on the indicating meter or the cathode-ray oscilloscope display tube. It may be necessary to use a high-pass filter in order to reduce room noise and spurious vibrations. The indicating meter may be a voltmeter, microammeter or oscilloscope. An oscilloscope is recommended because it enables the operator to positively identify resonances, including higher order harmonics, by Lissajous figure analysis.

6.1.3 *Specimen Supports*—The supports shall permit the specimen to oscillate without significant restriction in the desired mode. This is accomplished for all modes by supporting the specimen at its transverse fundamental nodal points ( $0.224 L$  from each end). The supports should have minimal area in contact with the specimen and shall be of cork, rubber, or similar material. In order to properly identify resonant frequencies, the receiver record pickup cartridge must be movable along the total specimen length. Provisions shall be made to adjust contact pressures of both record pickup cartridges in order to accommodate specimen size variations. The entire specimen support structure shall be mounted on a massive base plate resting on vibration isolators.

7.3 *Signal Pickup*—Signal detection can be via transducers in direct contact with the specimen or by non-contact transducers. Contact transducers are commonly accelerometers using piezoelectric or strain gage methods to measure the vibration. Non-contact transducers are commonly acoustic microphones, but they may also use laser, magnetic, or capacitance methods to measure the vibration. The frequency range of the transducer shall be sufficient to measure the expected frequencies of the specimens of interest. A suitable range would be 100 Hz to 50 kHz for most graphite test specimens. (Smaller and stiffer specimens vibrate at higher frequencies.) The frequency response of the transducer across the frequency range of interest shall have a bandwidth of at least 10 % of the maximum measured frequency before -3 dB power loss occurs.

7.4 *Electronic System*—The electronic system consists of a signal conditioner/amplifier, signal analyzer, and a frequency readout device. The system should have accuracy and precision sufficient to measure the frequencies of interest to an accuracy of 0.1 %. The signal conditioner/amplifier should be suitable to power the transducer and provide an appropriate amplified signal to the signal analyzer. The signal analysis system consists of a frequency counting device and a readout device. Appropriate devices are frequency counter systems with storage capability or digital storage oscilloscopes with a frequency counter module. With the digital storage oscilloscope, a Fast Fourier Transform signal analysis system may be useful for analyzing more complex waveforms and identifying the fundamental resonant frequency.

7.5 *Support System*—The support shall serve to isolate the specimen from extraneous vibration without restricting the desired mode of specimen vibration. Appropriate materials should be stable at the test temperatures. Support materials can be either soft or rigid for ambient conditions. Examples of soft materials would be a compliant elastomeric material, such as polyurethane foam strips. Such foam strips would have simple flat surfaces for the specimen to rest on. Rigid materials, such as metal or ceramic, should have sharp knife edges or cylindrical surfaces on which the specimen should rest. The rigid supports should be resting on isolation pads to prevent ambient vibrations from being picked up by the transducer. Wire suspension can also be used. Specimens shall be supported along node lines appropriate for the desired vibration in the locations described in Section 9.

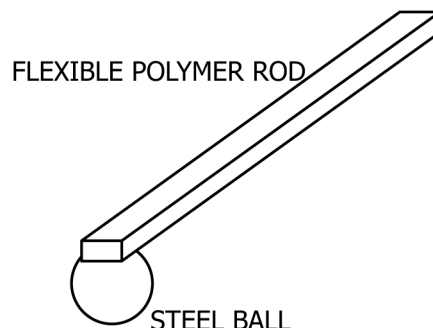


FIG. 2 - Schematic Diagram of Typical Dynamic Elastic Modulus Detection Apparatus Impulser for Small Specimens

## 8. Test Specimens

8.1 The specimens shall be prepared so that they are either rectangular or circular in cross-section. Either geometry can be used to measure both dynamic Young's modulus and dynamic shear modulus. Although the equations for computing shear modulus with a cylindrical specimen are both simpler and more accurate than those used with a rectangular bar, experimental difficulties in obtaining torsional resonant frequencies for a cylindrical specimen usually preclude its use for determining shear modulus.

8.2 Resonant frequencies for a given specimen are functions of the specimen dimensions as well as its mass and moduli. Dimensions should therefore be selected with this relationship in mind. The selection of size shall be made so that, for an estimated modulus, the resonant frequencies measured will fall within the range of frequency response of the transducers and electronics used. For a slender rod, the ratio of length to minimum cross-sectional dimension should have a value of at least 5. However, a ratio of approximately 10 to 20 is preferred for ease in exciting the fundamental frequency. For shear modulus measurements of rectangular bars, a ratio of width to thickness of 5 or greater is recommended for minimizing experimental difficulties.

8.3 *Selection and Preparation of Specimens*—In the selection and preparation of test specimens, take special care to obtain representative specimens that are straight, uniform in cross section, and free of extraneous liquids. Deviations from the recommended sample ratio range introduce an elevated level of difficulty in obtaining a recorded measurement for fundamental frequency that the operator can have confidence in. For this reason, it is recommended that two additional guidelines be employed as allowable in order to increase the likely accuracy of the frequency being recorded:

8.3.1 Determine the fundamental frequency using specimens that are within the recommended length to width ratio of between 5 and 20, or use progressively larger specimens as necessary, in order to establish baseline frequency characteristics of the material being evaluated. The expected value for fundamental frequency of a non-standard specimen can be calculated based upon the measured geometry and the known fundamental frequency of a standard specimen, and any deviation or shift can be appropriately noted.

8.3.2 Spurious vibration modes are more easily discounted if the test is repeated on the same specimen until ten readings are obtained that lie within  $\pm 10\%$  of the mean. It is acknowledged that for less ideal specimen geometries, the frequency mean that is eventually used for the modulus calculation may require an extended number of measurements until an appropriate group of ten readings is obtained. Operator experience will play a valuable role in the collection of resonant frequency values in non-standard specimen geometries.

8.4 All surfaces on the rectangular specimen shall be flat. Opposite surfaces across the length and width shall be parallel within 0.05 mm or 0.1 %, whichever is greater. Opposite surfaces across the thickness shall be parallel within 0.05 mm or 0.1 %, whichever is greater. The cylindrical specimen shall be round and constant in diameter within 0.05 mm or 0.1 %, whichever is greater.

8.5 Test specimen mass shall be determined within 0.1 % or 10 mg, whichever is greater.

8.6 *Measurement of Weight and Dimensions*—Determine the weight and the average length of the specimens within  $\pm 0.5\%$ . Determine average specimen cross-sectional dimension within  $\pm 1\%$ . Test specimen length shall be measured to within 0.025 mm or 0.1 %, whichever is greater. Test specimen cross-sectional dimensions (thickness and width in rectangular beams; diameter in cylindrical rods) shall be measured within 0.1% or 0.025 mm, whichever is greater, at three equally spaced locations along the length and an average value determined.

8.7 Porous materials and those susceptible to hydration should be dried in air at 120 °C in a drying oven until the mass is constant (less than 0.1 % or 10 mg difference in measured mass with 30 min of additional drying).

8.8 *Limitations on Dimensional Ratio*—Specimens having either very small or very large ratios of length to thickness may be difficult to excite in the fundamental modes of vibration. For this method, the ratio must be between 5 and 20 (slender rod limitations). It is recommended that the laboratory obtain and maintain an internal reference specimen with known and recorded fundamental resonant frequencies in flexure and torsion. The reference specimen should be used to check and confirm the operation of the test system on a regular basis. It can also be used to train operators in the proper test setup and test procedure. The reference specimen can be a standard ceramic material (alumina, silicon carbide, zirconia, etc.) or it may be of a similar size, composition, and microstructure to the types of specimens commonly tested at the laboratory. The reference specimen must meet the size, dimensional tolerances, and surface finish requirements of Section 8.

## 9. Procedure

9.1 Switch on/Activate all electrical equipment and allow to stabilize in accordance with the manufacturers' recommendations. (Use of a metal bar as a calibration standard is recommended to check equipment response and accuracy. Dimensional measurements and weight shall meet the requirements of it to stabilize according to the manufacturer's recommendations. 7.2.)

9.2 Use a test specimen established as a verification/calibration standard to verify the equipment response and accuracy.

9.3 *Fundamental Flexural Resonance Frequency (Out-of-Plane Flexure):*

9.3.1 Place the specimen on the supports located at the fundamental nodal points (0.224 L from each end; see Fig. 3).

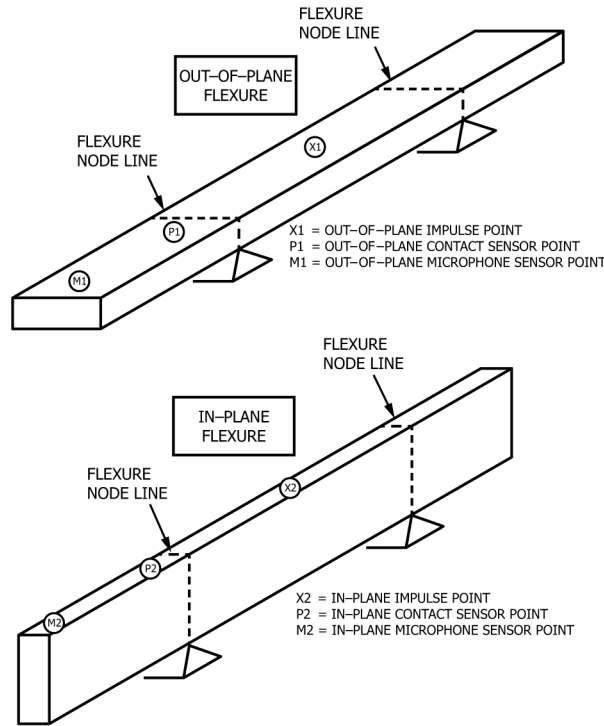


FIG. 3 Nodal Points Dynamic Modulus Tracking Guide Template Rectangular Specimens Tested for In-plane and Out-of-plane Flexure

9.3.2 Determine the direction of maximum sensitivity for the transducer. Orient the transducer so that it will detect the desired vibration.

9.3.2.1 *Direct Contact Transducers*—Place the transducer in contact with the test specimen to pick up the desired vibration. If the transducer is placed at an antinode (location of maximum displacement), it may mass load the specimen and modify the natural vibration. The transducer should preferably be placed only as far from the nodal points as necessary to obtain a reading (see Fig. 3). This location will minimize the damping effect from the contacting transducer. The transducer contact force should be consistent, with good response and minimal interference with the free vibration of the specimen.

9.3.2.2 *Non-Contact Transducers*—Place the non-contact transducer over an antinode point and close enough to the test specimen to pick up the desired vibration, but not so close as to interfere with the free vibration (see Fig. 3).

9.3.3 Strike the specimen lightly and elastically, either at the center of the specimen or at the opposite end of the specimen from the detecting transducer (see Fig. 3).

9.3.4 Record the resultant reading, and repeat the test until a recommended ten readings are obtained that lie within 10 % of the mean. The round-robin interlaboratory study (12.2) showed that data points significantly (>10 %) out of range were measurements of spurious vibration modes or secondary harmonics. If ten readings cannot be taken, a minimum of five readings that lie within 10 % of the mean shall be required for estimating the mean. Use the mean of these readings to determine the fundamental resonant frequency in flexure.

9.4 *Fundamental Flexural Resonance Frequency (In-Plane Flexure):*

9.4.1 This procedure is the same as that above (9.3), except that the direction of vibration is in the major plane of the specimen. Rotate the test bar 90° around its long axis and reposition it on the specimen supports (see Fig. 3). Transpose the width and thickness dimensions in the calculations. For homogeneous, isotropic materials, the calculated moduli should be the same as the moduli calculated from the out-of-plane frequency. The comparison of in-plane and out-of-plane frequency measurements can thus be used as a cross check of experimental methods and calculations.

9.5 *Transverse-Fundamental Torsional Resonance Frequency:*

9.5.1 PlaceSupport the specimen on the supports, which are located at the fundamental transverse nodal points (0.224 at the midpoint L from each end). Place the driving and pickup unit vibrating needles on the specimen center line at its extreme opposite ends with a minimal contact pressure consistent with good response. The vibrating direction of the driving and pickup needles must be perpendicular to the length of the specimen (of its length and width (the torsional nodal planes) (see Fig. 14(.b)).

8.2.2 Force the test specimen to vibrate at various frequencies and simultaneously observe the amplified output on an indicating meter or oscilloscope. Record the frequency of vibration of the specimen that results in a maximum displacement, having a well-defined peak on the indicator, where nodal point tracking indicates fundamental transverse resonance.

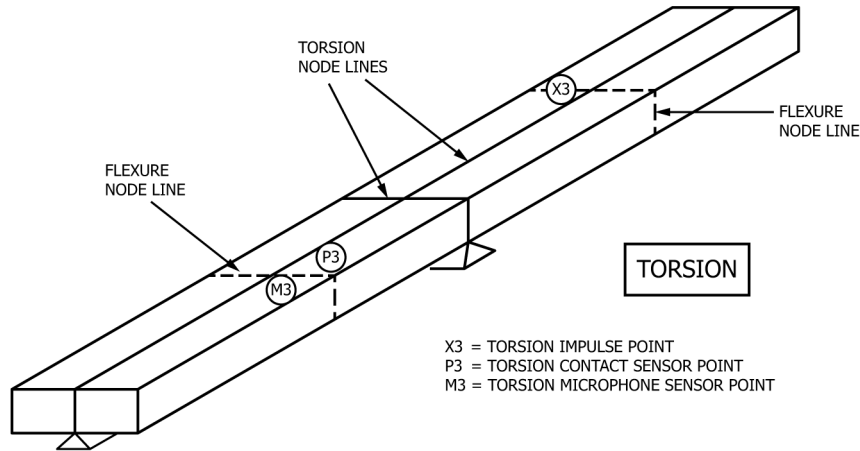


FIG. 4 Rectangular Specimen Tested for Torsional Vibration

8.2.3 A basic understanding of Lissajous patterns as displayed on an oscilloscope cathode ray tube (CRT), will aid in the proper identification of the modes of vibration and harmonic frequencies observed. As the oscillator frequency level is increased from a point well below expected resonance, a single closed loop Lissajous pattern tilted from the horizontal reference plane, will eventually be displayed on the CRT. This pattern denotes a resonance mode. The nodal points dynamic modulus tracking guide template (Fig. 3) may be used to identify any resonant mode.

9.5.2 Move the pickup cartridge needle slowly. Locate the transducer at one quadrant of the specimen, preferably at approximately 0.224 *L* toward the specimen center and observe the Lissajous pattern loop. Fundamental transverse resonance is indicated from one end and toward the edge. This location is a nodal point of flexural vibration and will minimize the possibility of detecting a spurious flexural mode (see Fig. 4 when the following conditions prevail:-).

8.2.4.1 The loop pattern flattens to a horizontal line with the pickup needle over the specimen support.

8.2.4.2 The CRT pattern opens up to a full loop in a direction normal to its original direction, with the pickup needle over the specimen center.

8.2.5 Return the pickup needle to its original position at the specimen end.

9.5.3 Spurious resonating frequency modes may mask or attenuate the fundamental transverse frequency indication. Investigation of higher order harmonic resonating frequencies by use of the tracking guide template ( Strike the specimen on the quadrant diagonally opposite Fig. 3) will help to identify the correct fundamental frequency mode. the transducer, again at 0.224 *AL* plot of the ratio of harmonic to fundamental frequency for transverse from the end and near the edge. Striking at a flexural nodal point will minimize the possibility of exciting a flexural mode of vibration ((see Fig. 4) Fig. 4 may then be used to calculate the fundamental transverse resonant frequency mode:-).

9.5.4 Record the resultant reading, and repeat the test until a recommended ten readings are obtained that lie within 10 % of the mean. The round-robin interlaboratory study (12.2) showed that data points significantly (> 10 %) out of range were measurements of spurious vibration modes or secondary harmonics. If ten readings cannot be taken, a minimum of five readings that lie within 10 % of the mean shall be required for estimating the mean. Use the mean of these readings to determine the fundamental resonant frequency in torsion.

#### 9.6 Longitudinal Fundamental Resonance Frequency:-Frequency—

8.3.1 Leave the specimen supported at the fundamental transverse mode nodal points as in 8.2.1. Rotate the driving unit and pickup cartridge needles so as to induce vibrations parallel to the specimen length (Fig. 1(a)). This procedure is the same as that above (9.3), except that the direction of vibration is longitudinal along the long axis of the specimen. However, the specimen should be supported at locations other than their nodal points, as this will encourage the specimen to vibrate in the flexural mode in addition to the longitudinal mode. Place either a contacting or non-contacting transducer at one end of the specimen and strike the opposite end to induce a vibration parallel to the specimen length. For homogeneous, isotropic materials, the calculated moduli should be the same as the moduli calculated from the in-plane and out-of-plane frequency. A comparison to the in-plane and out-of-plane modulus can thus be used as a cross check of experimental methods and calculations.

8.3.2 Force the test specimen to vibrate as in 8.2.2. Record the frequency of vibration of the test specimen, where nodal point tracking indicates fundamental longitudinal resonance. The second harmonic longitudinal resonant frequency is twice the fundamental longitudinal resonant frequency.

#### 8.4 Torsional Fundamental Resonance Frequency:

8.4.1 Leave the specimen supported as in 8.2.1. Rotate the driving unit and pickup cartridge needles so as to induce vibrations perpendicular to the length of the sample (Fig. 1 (d)).



8.4.2 Force the specimen to vibrate as in 8.2.2. Record the frequency of vibration of the test specimen, where nodal point tracking indicates fundamental torsional resonance. The second harmonic torsional resonant frequency is twice the fundamental torsional resonant frequency.

## 10. Calculation

10.1 Calculate the dynamic modulus of elasticity for the transverse or flexural mode of vibration from the fundamental transverse frequency, weight, and dimensions of the test specimen as follows:

$$\text{Dynamic } E = CMf^2 \quad (4)$$

*Dynamic Young's Modulus*<sup>3,4</sup>:

where units are as defined in 4.1.1. The evaluation of the constant  $C$ , because of the complexity of its determination, is in tabular form. Eq 4 may be rewritten in the forms:

$$\text{Dynamic } E \text{ (pascals)} = A_c M f^2 / d \text{ for rods with} \quad (5)$$

circular cross sections

10.1.1 For the fundamental flexure frequency of a rectangular bar,

$$E = 0.9464(mf_f^2/b)(L^3/t^3)T_1 \quad (2)$$

where:

- $E$  = Young's modulus, Pa,
- $m$  = mass of the bar, g (see Note 2),
- $b$  = width of the bar, mm (see Note 1 and Note 2),
- $L$  = length of the bar, mm, (see Note 2),
- $t$  = thickness of the bar, mm (see Note 1 and Note 2),
- $\mu$  = Poisson's Ratio,
- $f_f$  = fundamental resonant frequency of bar in flexure, Hz, and
- $T_1$  = correction factor for fundamental flexural mode to account for finite thickness of bar, Poisson's ratio, and so forth.

$$T_1 = 1 + 6.585(1 + 0.0752\mu + 0.8109\mu^2)\left(\frac{t}{L}\right)^2 - 0.868\left(\frac{t}{L}\right)^4 \left[ \frac{8.340(1 + 0.2023\mu + 2.173\mu^2)\left(\frac{t}{L}\right)^4}{1.000 + 6.338(1 + 0.1408\mu + 1.536\mu^2)\left(\frac{t}{L}\right)^2} \right] \quad (3)$$

NOTE 1—The width ( $b$ ) and thickness ( $t$ ) values used in the modulus calculations (Eq 2 and Eq 3) for the rectangular specimens will depend on the type of vibration (out-of-plane or in-plane) induced in the specimen. The cross-sectional dimension  $t$  will always be parallel to the vibrational motion. The dimension  $b$  will always be perpendicular to the vibrational motion. In effect, the two different flexural modes will give two different fundamental resonant frequencies, but the calculations for the two modes should give the same modulus value, because the values for  $b$  and  $t$  are exchanged in the calculations for the two different flexure modes.

NOTE 2—In the modulus equations, the mass and length terms are given in units of grams and millimeters. However, the defined equations can also be used with mass and length terms in units of kilograms and meters with no changes in terms or exponents.

10.1.1.1 If  $L/t \geq 10$ ,  $T_1$  can be simplified to the following:

$$T_1 = 1.000 + 6.585(t/L)^2 \quad (4)$$

and  $E$  can be calculated directly.

10.1.1.2 If  $L/t < 10$  and Poisson's ratio is known, then  $T_1$  can be calculated directly from Eq 3 and then used to calculate  $E$ .

10.1.1.3 If  $L/t < 10$  and Poisson's ratio is not known, then an initial Poisson's ratio must be assumed to begin the computations. An iterative process is then used to determine a value of Poisson's ratio, based on experimental Young's modulus and shear modulus. The iterative process is flowcharted in Fig. 5 and described in (1) through (5) below.

(1) Determine the fundamental flexural and torsional resonant frequency of the rectangular test specimen, as described in Section 9. Using Eq 9 and Eq 10, calculate the dynamic shear modulus of the test specimen for the fundamental torsional resonant frequency.

(2) Using Eq 2 and Eq 3, calculate the dynamic Young's modulus of the rectangular test specimen from the fundamental flexural resonant frequency, dimensions and mass of the specimen, and initial/iterative Poisson's ratio. Care shall be exercised in using consistent units for all of the parameters throughout the computations.

(3) Substitute the dynamic shear modulus and Young's modulus values calculated in steps (1) and (2) into Eq 12 for Poisson's ratio satisfying isotropic conditions. Calculate a new value for Poisson's ratio for another iteration beginning at Step (2).

<sup>3</sup> Spinner, S., Reichard, T. W., and Tefft, W. E., "A Comparison of Experimental and Theoretical Relations Between Young's Modulus and the Flexural and Longitudinal Resonance Frequencies of Uniform Bars," *Journal of Research of the National Bureau of Standards-A. Physics and Chemistry*, Vol 64A, No. 2, March-April, 1960.

<sup>4</sup> Spinner, S., and Tefft, W. E., "A Method for Determining Mechanical Resonance Frequencies and for Calculating Elastic Moduli from These Frequencies," Proceedings, ASTM, 1961, pp. 1221-1238

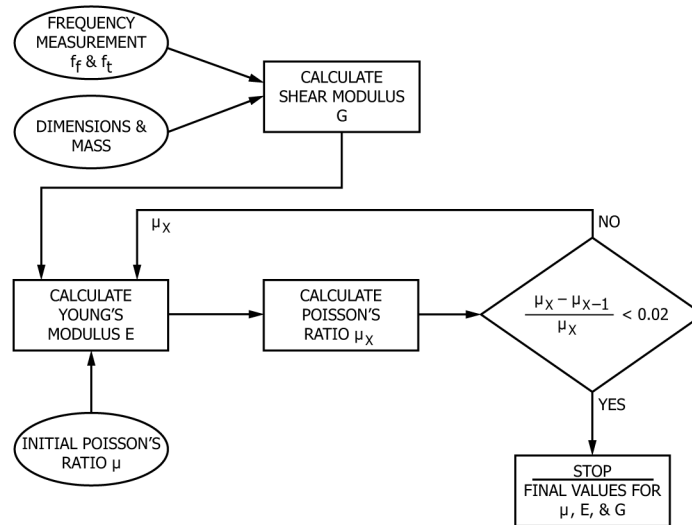


FIG. 5 Process Flowchart for Iterative Determination of Poisson's Ratio

(4) Repeat Steps (2) and (3) until no significant difference (2 % or less) is observed between the last iterative value and the final computed value of the Poisson's ratio.

(5) Self-consistent values for the moduli are thus obtained.

where  $d$  is the diameter of the rod in metres, and

$$\text{Dynamic } E \text{ (pascals)} = A_R M f^2 / w \text{ for bars with} \quad (6)$$

square or rectangular cross-sections

where  $w$  is the width dimension of the bar in metres.

10.1.2 Values of  $A_e$  and  $A_R$  are shown in Annex A1 under Table A1.1 and Table A1.2. The value of  $A_e$  is given as a function of the diameter-to-length ratio of the sample. The value of the fundamental flexural frequency of  $A_R$  is given as a function of the ratio rod of circular cross-section<sup>3</sup> of:

$$E = 1.6067 \left( \frac{L^3}{D^4} \right) (m f_f^2) T_1 \quad (5)$$

where: <https://standards.iteh.ai/catalog/standards/sist/6259dd19-70e1-4798-8025-c6aa33c5a4d6/astm-c747-16>

$D$  = diameter of rod, mm (see Note 2), and

$T_1$  = correction factor for fundamental flexural mode to account for finite diameter of bar, Poisson's ratio, and so forth.

The dimension in the direction of vibration,  $t$ , to the length. The dimension,  $w$ , is perpendicular to the vibration direction, as shown in Fig. 5. Table A1.1 and Table A1.2 have been calculated for three values of Poisson's ratio ( $\mu$ ). The value of ( $\mu$ ) = 1/6 is normally used for carbon-graphite materials:

$$T_1 = 1 + 4.939(1 + 0.0752\mu + 0.8109\mu^2) \left( \frac{D}{L} \right)^2 - 0.4883 \left( \frac{D}{L} \right)^4 - \left[ \frac{4.691 \left( 1 + 0.2023\mu + 2.173\mu^2 \left( \frac{D}{L} \right)^4 \right)}{1.000 + 4.754 \left( 1 + 0.1408\mu + 1.536\mu^2 \left( \frac{D}{L} \right)^2 \right)} \right] \quad (6)$$

10.1.2.1 If  $L/D \geq 10$ , then  $T_1$  can be simplified to the following:

$$T_1 = 1.000 + 4.939(D/L)^2 \quad (7)$$

10.1.2.2 If  $L/D < 10$  and Poisson's ratio is known, then  $T_1$  can be calculated directly from Eq 6 and then used to calculate  $E$ .

10.1.2.3 If  $L/D < 10$  and Poisson's ratio is not known, then an initial Poisson's ratio must be assumed to start the computations. Final values for Poisson's ratio, dynamic Young's modulus, and dynamic shear modulus are determined, using the same method shown in Fig. 5 and described in (1) through (5) in 10.1.1.3, but using the modulus equations for circular bars (Eq 5, Eq 6, and Eq 7).

10.1.3 For the fundamental longitudinal frequency of a rectangular or circular bar:

$$E = 4.000 f_l^2 L^2 \rho \quad (8)$$

where:

$f_l$  = fundamental resonant frequency of bar vibrating longitudinally, Hz, and