



## Designation: ~~E787 – 81 (Reapproved 2011)~~ E787 – 81 (Reapproved 2017)

# Standard Specification for Disposable Glass Micro Blood Collection Pipets<sup>1</sup>

This standard is issued under the fixed designation E787; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

*This standard has been approved for use by agencies of the U.S. Department of Defense.*

## 1. Scope

1.1 This specification covers two dimensionally different disposable glass micropipets used primarily to collect whole human blood specimens for clinical analysis and testing. They are available as coated with heparin or uncoated.

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

[E438 Specification for Glasses in Laboratory Apparatus](#)

## 3. Terminology

3.1 *Definitions of Terms Specific to This Standard:*

3.1.1 *disposable micropipets*—in accordance with this specification and the expected product performance expressed in this standard, those pipets which are to be used one time only. *Any institution or individual who reuses a disposable pipet must bear full responsibility for its safety and effectiveness.*

## 4. Classification

4.1 This specification covers two dimensionally different disposable glass pipets as follows:

4.1.1 *Short Pipet*—Approximately 75 mm long and coated with heparin (Type I) or uncoated (Type II). These are commercially recognized as Caraway pipets.<sup>3</sup>

4.1.2 *Long Pipet*—Approximately 150 mm long and coated with heparin (Type I) or uncoated (Type II). These are commercially recognized as Natelson pipets.<sup>4</sup>

## 5. Materials and Manufacture

5.1 *Glass*—The pipets shall be fabricated from borosilicate glass, Type I, Class B, or soda lime glass, Type II, in accordance with Specification [E438](#).

5.2 *Heparin*—shall be the ammonium salt isolated from the lungs or intestinal mucosa of beef or pork origin. The heparin potency shall be 1 mg of ammonium heparin compound which is equal to at least 100 USP units.<sup>5</sup>

## 6. Physical Requirements

6.1 *Design*—The disposable glass micro blood collection pipets, both short and long, shall be straight and pulled to a tapered point at one end. Any cross section of the pipets, taken in a plane perpendicular to the longitudinal axis, shall be circular. The pipets shall be lightly firepolished at both ends with no run-in and possess color bands to denote presence or absence of heparin content.

6.2 *Dimensions:*

6.2.1 The short Caraway pipet shall be approximately 75 mm long and 4 mm in outside diameter. The pipet shall hold a liquid volume of 310 to 470  $\mu$ L. The tapered point length and tip orifice opening shall be as specified in [Fig. 1](#).

<sup>1</sup> This specification is under the jurisdiction of ASTM Committee E41 on Laboratory Apparatus and is the direct responsibility of Subcommittee E41.01 on Apparatus Laboratory Ware and Supplies.

Current edition approved Dec. 1, 2011; Jan. 1, 2017. Published December 2011/February 2017. Originally approved in 1981. Last previous edition approved in 2006/2011 as E787 – 81 (2006)(2011).<sup>1</sup> DOI: 10.1520/E0787-81R11-10.1520/E0787-81R17.


<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>3</sup> Caraway, W. T., and Fanger, H., "Ultramicro Procedures In Clinical Chemistry," *American Journal of Clinical Pathology*, 25, 1955, pp. 316–331.

<sup>4</sup> Natelson, S., Ph.D., *Micro-Techniques of Clinical Chemistry*, Charles C. Thomas, Springfield, Ill., 1961, p. 70.

<sup>5</sup> *The United States Pharmacopeia*, 19th Revision, pp. 229–230.

NOT TO SCALE

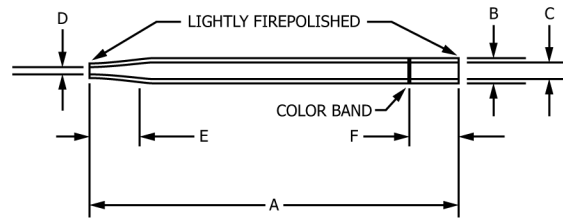

Capacity: 310 to 470  $\mu$ L  
 Coding: Red band-heparin-coated (Type I)  
 Blue band-uncoated (Type II)

Dimensions in millimetres

A	Overall length	73–77
B	Outside diameter	3.90–4.20
C	Inside diameter	2.40–2.80
D	Inside tip diameter	0.70–1.50
E	Length of taper	6–12
F	Color band location	0–10

FIG. 1 Caraway Pipet


6.2.2 The long Natelson pipet shall be approximately 150 mm long and 3 mm in outside diameter. The pipet shall hold a liquid volume of 220 to 420  $\mu$ L. The tapered point length and tip orifice opening shall be as specified in Fig. 2.

6.3 *Workmanship*—The pipets, as illustrated in Fig. 1 and Fig. 2, shall be free of defects that noticeably detract from their appearance or impair their serviceability. They shall be free of lint, or significant foreign matter, loose or embedded when viewed under normal room lighting. The top and tip ends of the pipets shall be cut at approximately 90° to the pipet axis and shall not be cracked or have jagged ends or chips that enter the bore of the pipet.

6.4 *Color Coding*—Each disposable glass micro blood collection pipet shall be color-coded to identify the pipet. The heparin-coated pipet (Type 1) shall have a red color band. The uncoated pipet (Type 2) shall have a blue color band. The location of these color bands shall be as specified in Fig. 1 and Fig. 2.

<https://standards.iteh.ai/catalog/standards/astm/83197703-dc6b-4c08-8c35-9c42fde3ea8f/astm-e787-812017>

NOT TO SCALE

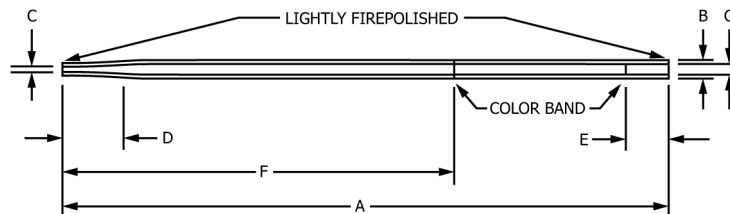

Capacity: 220 to 420  $\mu$ L  
 Coding: Red band-heparin-coated (Type I)  
 Blue band-uncoated (Type II)

Dimensions in millimetres

A	Overall length	145–155
B	Outside diameter	2.80–3.10
C	Inside tip diameter	0.75–1.30
D	Length of taper	6–12
E	Color band location	0–10 top
F	Alternative location	100 $\pm$ 1 from tip
G	Inside diameter	1.30–1.80

FIG. 2 Natelson Pipet