This document is not an ASTM standard and is intended only to provide the user of an ASTM standard an indication of what changes have been made to the previous version. Because it may not be technically possible to adequately depict all changes accurately, ASTM recommends that users consult prior editions as appropriate. In all cases only the current version of the standard as published by ASTM is to be considered the official document.



Designation: F2070 - 00 (Reapproved 2011) F2070 - 00 (Reapproved 2017) American National Standard

Standard Specification for Transducers, Pressure and Differential, Pressure, Electrical and Fiber-Optic¹

This standard is issued under the fixed designation F2070; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ε) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This specification covers the requirements for pressure and differential pressure transducers for general applications.

1.2 Special requirements for naval shipboard applications are included in Supplementary Requirements S1, S2, and S3.

1.3 The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only. <u>mathematical conversions to inch-pound units that are provided for information only and are not considered standard.</u> Where information is to be specified, it shall be stated in SI units.

1.4 This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices, safety, health and environmental practices and determine the applicability of regulatory limitations prior to use.

1.4 Special requirements for naval shipboard applications are included in Supplementary Requirements S1, S2, and S3.

1.5 This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.

2. Referenced Documents

2.1 ASTM Standards:²

D3951 Practice for Commercial Packaging

2.2 ANSI/ISA Standards:³

ANSI/ISA S37.1 Electrical Transducer Nomenclature and Terminology

2.3 ISO Standard: Standards:⁴

ISO 9001 Quality System—Model for Quality Assurance in Design/Development, Production, Installation, and Servicing

3. Terminology

3.1 Terms marked with (ANSI/ISA S37.1)"ANSI/ISA S37.1" are taken directly from ANSI/ISA S37.1 (R-1982) and are included for the convenience of the user.

3.2 Definitions:

3.2.1 Terminology consistent with ANSI/ISA S37.1 shall apply, except as modified by the definitions listed as follows:

3.2.2 *absolute pressure_pressure*, *n*_pressure measured relative to zero pressure (vacuum). (ANSI/ISA S37.1)ANSI/ISA S37.1)ANSI/ISA S37.1)

3.2.3 *ambient <u>conditions</u>* conditions such as pressure and temperature of the medium surrounding the case of (ANSI/ISA S37.1)ANSI/ISA S37.1)ANSI/ISA S37.1

Copyright © ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959. United States

¹ This specification is under the jurisdiction of ASTM Committee F25 on Ships and Marine Technology and is the direct responsibility of Subcommittee F25.10 on Electrical.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For Annual Book of ASTM Standards volume information, refer to the standard's Document Summary page on the ASTM website.

³ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, http://www.ansi.org.

⁴ Available from International Organization for Standardization (ISO), 1 rue de Varembé, Case postale 56, CH-1211, Geneva 20, Switzerland. <u>ISO Central Secretariat</u>, BIBC II, Chemin de Blandonnet 8, CP 401, 1214 Vernier, Geneva, Switzerland, http://www.iso.org.

3.2.4 *burst <u>pressure</u>_pressure, n*_the maximum pressure applied to the transducer sensing element without rupture of the sensing element or transducer case as specified.

3.2.5 *calibration*—*calibration*, *n*—the test during which known values of measurands are applied to the transducer and corresponding output readings are recorded under specified conditions. (ANSI/ISA S37.1)ANSI/ISA S37.1

3.2.6 *common mode pressure*—*pressure*, *n*—the common mode pressure is static line pressure applied simultaneously to both pressure sides of the transducer for the differential pressure transducer only.

3.2.7 *differential <u>pressure pressure</u>*, <u>n</u>-the difference in pressure between two points of measurement. (ANSI/ISA S37.1) ANSI/ISA S37.1)

3.2.8 *environmental <u>conditions</u>*—<u>conditions</u>, <u>n</u>—specified external conditions, such as shock, vibration, and temperature, to which a transducer may be exposed during shipping, storage, handling, and operation. (ANSI/ISA S37.1)ANSI/ISA S37.1

3.2.9 *error*—*error*, *n*—the algebraic difference between the indicated value and the true value of the measurand.

(ANSI/ISA S37.1)ANSI/ISA S37.1

3.2.10 *fiber-optic pressure transducer*—<u>transducer</u>, <u>n</u>—a device that converts fluid pressure, by means of changes in fiber-optic properties, to an output that is a function of the applied measurand. The fiber-optic pressure transducer normally consists of a sensor head, optoelectronics module, and connectorized fiber-optic cable.

3.2.11 *hysteresis*—*hysteresis*, *n*—the maximum difference in output, at any measurand value within the specified range, when the value is approached first with increasing and then with decreasing measurand. (ANSI/ISA S37.1)ANSI/ISA S37.1

3.2.12 *insulation resistance*—*resistance*, *n*—the resistance measured between insulated portions of a transducer and between the insulated portions of a transducer and ground when a specified dc voltage is applied under specified conditions.

3.2.13 *line pressure*—*pressure*, *n*—the pressure relative to which a differential pressure transducer measures pressure.

(ANSI/ISA S37.1)ANSI/ISA S37.1

3.2.14 *operating environmental conditions—conditions, n—* environmental conditions during exposure to which a transducer must perform in some specified manner.

(ANSI/ISA S37.1)ANSI/ISA S37.1

3.2.15 optical—optical, adj—involving the use of light-sensitive devices to acquire information.

3.2.16 *optical fiber*—*fiber, n*—a very thin filament or fiber, made of dielectric materials, that is enclosed by material of lower index of refraction and transmits light throughout its length by internal reflections.

3.2.17 *optoelectronics module_module, n_*a component of the fiber-optic pressure transducer that contains the optical source and detector, and signal conditioner devices necessary to convert the sensed pressure to the specified output signal.

3.2.18 *output—output, n*_electrical or numerical quantity, produced by a transducer or measurement system, that is a function of the applied measurand.

3.2.19 *overpressure*—<u>overpressure</u>, <u>n</u>—the maximum magnitude of measurand that can be applied to a transducer without causing a change in performance beyond the specified tolerance.

3.2.20 *pressure cycling—cycling, n*—the specified minimum number of specified periodic pressure changes over which a transducer will operate and meet the specified performance.

3.2.21 pressure rating—rating, n—the maximum allowable applied pressure of a differential pressure transducer.

3.2.22 process medium-medium, n-the measured fluid (measurand) that comes in contact with the sensing element.

3.2.23 *range*<u>range</u>, <u>n</u><u>measurand</u> values, over which a transducer is intended to measure, specified by their upper and lower (ANSI/ISA S37.1)<u>ANSI/ISA S37.1</u>)

3.2.24 *repeatability*—*repeatability*, *n*—ability of a transducer to reproduce output readings when the same measurand value is applied to it consecutively, under the same conditions, and in the same direction. (ANSI/ISA S37.1)ANSI/ISA S37.1

3.2.25 *response*—*response*, *n*—the measured output of a transducer to a specified change in measurand.

3.2.26 *ripple*—*ripple*, *n*—the peak-to-peak ac component of the dc output.

3.2.27 sensing <u>element</u>—<u>element</u>, <u>n</u>—that part of the transducer that responds directly to the measurand. (ANSI/ISA S37.1) ANSI/ISA S37.1)

3.2.28 sensitivity factor—factor, n—the ratio of the change in transducer output to a change in the value of the measurand.

3.2.29 sensor <u>head</u>—<u>head</u>, <u>n</u>—the transduction element of the fiber-optic pressure transducer that detects fluid pressure by means of changes in optical properties.

3.2.30 *signal <u>conditioner</u>_conditioner, n_*an electronic device that makes the output signal from a transduction element compatible with a readout system.

3.2.31 *static error band*—*band*, *n*—static error band is the maximum deviation from a straight line drawn through the coordinates of the lower range limit at specified transducer output, and the upper range limit at specified transducer output expressed in percent of transducer span.

3.2.32 *transducer*<u>transducer</u>, <u>n</u>device that provides a usable output in response to a specified measurand. (ANSI/ISA S37.1)ANSI/ISA S37.1

3.2.33 wetted parts-parts, n-transducer components with at least one surface in direct contact with the process medium.

4. Classification

4.1 *Designation*—Most transducer manufacturers use designations or systematic numbering or identifying codes. Once understood, these designations could aid the purchaser in quickly identifying the transducer type, range, application, and other parameters.

4.2 *Design*—Pressure transducers typically consist of a sensing element that is in contact with the process medium and a transduction element that modifies the signal from the sensing element to produce an electrical or optical output. Some parts of the transducer may be hermetically sealed if those parts are sensitive to and may be exposed to moisture. Pressure connections must be threaded with appropriate fittings to connect the transducer to standard pipe fittings or to other appropriate leak-proof fittings. The output cable must be securely fastened to the body of the transducer. A variety of sensing elements are used in pressure transducers. The most common elements are diaphragms, bellows, capsules, Bourdon tubes, and piezoelectric crystals. The function of the sensing element is to produce a measurable response to applied pressure or vacuum. The response may be sensed directly on the element or a separate sensor may be used to detect element response. The following is a brief introduction to the major pressure sensing technology design categories.

4.2.1 Electrical Pressure Transducers:

4.2.1.1 *Differential Transformer Transducer*—Linear variable differential transformers (LVDT) are variable reluctance devices. Pressure-induced sensor movement, usually transmitted through a mechanical linkage, moves a core within a differential transformer. Sensors are most commonly bellows, capsules, or Bourdon tubes. The movement of the core within the differential transformer results in a change in reluctance that translates to a voltage output. An amplifying mechanical linkage may be used to obtain adequate core movement.

4.2.1.2 *Potentiometric Transducer*—Pressure-induced movement of the sensing element causes movement of a potentiometer wiper resulting in a change in resistance which translates to a voltage output. A bellows or Bourdon tube is commonly used as the sensing element. An amplifying mechanical linkage may be used to obtain adequate wiper movement.

4.2.1.3 *Strain Gage Transducer*—Typical strain gage pressure transducers convert a pressure into a change in resistance due to strain which translates to a relative voltage output. Pressure-induced movement in the sensing element deforms strain elements. The strain elements of a typical strain gage pressure transducer are active arms of a Wheatstone Bridge arrangement. As pressure increases, the bridge becomes electrically unbalanced as a result of the deformation of the strain elements providing a change in voltage output.

4.2.1.4 Variable Capacitance Transducer—Variable capacitance pressure transducers sense changes in capacitance with changes in pressure. Typically, a diaphragm is positioned between two stator plates. Pressure-induced diaphragm deflection changes the circuit capacitance, which is detected and translated into a change in voltage output.

4.2.1.5 *Variable Reluctance Transducer*—Variable reluctance pressure transducers sense changes in reluctance with changes in pressure. Typically, a diaphragm is positioned between two ferric core coil sensors that when excited produce a magnetic field. Pressure-induced diaphragm deflection changes the reluctance, which is detected and translated to a change in voltage output.

4.2.1.6 *Piezoelectric Transducer*—Piezoelectric transducers consist of crystals made of quartz, tourmaline, or ceramic material. Pressure-induced changes in crystal electrical properties cause the crystal to produce an electrical output which is detected and translated to a change in voltage output.

4.2.2 Fiber-Optic Pressure Transducers:

4.2.2.1 *Fabry-Perot Interferometer*—Fabry-Perot interferometers (FPI) consist of two mirrors facing each other, the space between the mirrors being called the cavity length. Light reflected in the FPI is wavelength modulated in exact accordance with the cavity length. Pressure-induced movement of one of the mirrors causes a measurable change in cavity length and a phase change in the reflected light signal. This change is optically detected and processed.

4.2.2.2 *Bragg Grating Interferometer*—A Bragg grating is contained in a section about 1 cm long and acts as a narrow band filter that detects variation in the optical properties of the fiber. When the fiber is illuminated with an ordinary light source such as an LED, only a narrow band of light will be reflected back from the grating section of the fiber. If a pressure is applied to the grating section of the fiber, the grating period changes, and hence, the wavelength of the reflected light, which can be measured.

4.2.2.3 *Quartz Resonators*—Typically, a pair of quartz resonators are inside the pressure transducer. These are excited by the incoming optical signal. One resonator is load-sensitive and vibrates at a frequency determined by the applied pressure. The second resonator vibrates at a frequency that varies with the internal temperature of the transducer. Optical frequency signals from the resonators are transmitted back to the optoelectronics interface unit. The interface unit provides an output of temperature-compensated pressure.

4.2.2.4 *Micromachined Membrane/Diaphragm Deflection*—The sensing element is made on a silicon substrate using photolithographic micromachining. The deflection of this micromachined membrane is detected and measured using light. The light is delivered to the sensor head through an optical fiber. The light returning from the membrane is proportional to the pressure deflection of the membrane and is delivered back to a detector through an optical fiber. The fiber and the sensor head are packaged within a thin tubing.

4.3 *Types*—The following are common types of pressure and differential pressure transducers: pressure, differential; pressure (gage, absolute and sealed); pressure, vacuum; and pressure, compound.

4.4 *Process Medium*—The following are the most common types of process media: freshwater, oil, condensate, steam, nitrogen and other inert gases, seawater, flue gas and ammonia, and oxygen.

4.5 Application—The following is provided as a general comparison of different types of transducers and considerations for application.

4.5.1 *LVDT Transducer*—The sensor element may become complicated depending on the amount of motion required for core displacement. Careful consideration should be exercised when the application includes very low- or high-pressure measurement, overpressure exposure, or high levels of vibration. Careful consideration should also be exercised when measuring differential pressure of process media having high dielectric constants, especially liquid media. If the process media is allowed to enter the gap between the sensor element and core, accuracy may suffer. Frequency response may suffer depending on the type of mechanical linkage(s) used in the transducer.

4.5.2 *Potentiometric Pressure Transducer*—Potentiometric pressure transducers are generally less complicated than other designs. Careful consideration should be exercised when the application includes very low pressure measurement, overpressure exposure, high levels of vibration, stability and repeatability over extended periods of time, or extremely high resolution requirements. Frequency response may suffer depending on the type of mechanical linkage(s) used. Technological advances have yielded more reliable designs that are commonly used.

4.5.3 *Strain Gage Transducers*—Low-level output strain gage transducers are among the most common pressure transducers. They are available in very compact packages which lend well in applications in which size is critical. Strain gage transducers that demonstrate high degrees of accuracy and excellent frequency response characteristics are readily available. Careful consideration should be exercised when the application includes very low-pressure measurement, very low lag or delay, high vibration levels, extreme overpressure requirements, or critical stability over extended periods.

4.5.4 Variable Capacitance Transducers—Variable capacitance transducers are well suited to measure dry, clean gases at very low pressures with a high degree of accuracy. Careful consideration should be exercised when measuring differential pressure of process media having high dielectric constants, especially liquid media. If the process media is allowed to enter the gap between the diaphragm and stators, accuracy may suffer. Process media that alters the dielectric constant between the diaphragm and stators also alters the output of the transducer unless isolation devices such as membranes or oil fills are used.

4.5.5 Variable Reluctance Transducers—Variable reluctance transducers are well suited to measure most process media, especially if the core coil sensors are isolated from the process media. Variable reluctance transducers are well suited for applications that include high shock or vibration levels, extreme overpressure requirements, high degrees of accuracy, or critical stability over extended periods. Careful consideration should be exercised when evaluating size, weight, and cost. All reluctance devices are affected by strong magnetic fields.

4.5.6 *Piezoelectric Transducers*—Piezoelectric transducers are very effective in measuring changes in pressure. The piezoelectric crystals only produce an output when they experience a change in load. With adequate signal conditioners they can also be used to perform static measurements.

4.5.7 *Fiber-Optic Pressure Transducers*—Fiber-optic pressure transducers can be used in virtually all applications. They are extremely sensitive and are beneficial for high resolution measurements. They are unaffected by electromagnetic interference and are recommended in applications where EMI is a problem. These transducers are by nature intrinsically safe and are especially applicable for hazardous environments.

4.6 *Range*—Each manufacturer of transducers advertises a standard operating range for their offered selections but there is no industry-wide standard of specific ranges for transducers. Ranges are available that cover applications from vacuums to 210 MPaG (30 000 psig). Refer to individual manufacturer recommendations on range best suited to each application or specify an exact range if the range is a critical characteristic.

4.7 *Pressure Rating*—Pressure rating applies only to differential pressure transducers. Differential pressure transducers must be selected with a pressure rating for the maximum media pressure to be encountered. The purchaser should refer to specific manufacturer guidance to ensure a transducer has the proper pressure rating for each intended application.

4.8 *Power Supply*—Power supplies furnish excitation to the transducer. Power supplies may include batteries; line-powered, electronically regulated, dc power supplies; or ac power directly from the power system.

4.9 *Output*—Output signals can be electrical or optical dependent on design. Output must be measurable and must correspond with pressure applied within the range of the transducer. Multiple output signals shall be provided when specified. One signal shall be designated as the prime and the other as supplemental.

4.10 *Pressure Connection*—The pressure connection is the opening of the transducer used to allow the process medium to reach the sensing element. Differential pressure transducers have two pressure connections, a high-pressure port and a low-pressure port.

5. Ordering Information

5.1 The purchaser should provide the manufacturer with all of the pertinent application data shown in accordance with 5.2. If special application operating conditions exist that are not shown in the acquisition requirements, they should also be described.

5.2 Acquisition Requirements—Acquisition documents should specify the following:

- 5.2.1 Title, number, and date of this specification,
- 5.2.2 Manufacturer's part number,
- 5.2.3 Range, pressure rating (differential only), power supply, output,
- 5.2.4 Mounting method (see 7.2),
- 5.2.5 Type of pressure connection (see 7.5),
- 5.2.6 Type of electrical connection (see 7.4),
- 5.2.7 When an electrical connection mating plug is not to be provided (see 7.4),
- 5.2.8 System process medium,
- 5.2.9 Prime output signal,
- 5.2.10 Supplemental output signal, if required,
- 5.2.11 System operating characteristics, such as pressure and flow rate,
- 5.2.12 Materials,
- 5.2.13 Environmental requirements, such as vibration and ambient temperature,
- 5.2.14 Quantity of transducers required,
- 5.2.15 Size and weight restrictions (see 7.7),
- 5.2.16 Critical service life requirements (see 8.1),
- 5.2.17 Performance requirements (see 8.2),
- 5.2.18 Special surface finish requirements (see 9.1), Standards
- 5.2.19 Special cleaning requirements (see 9.2),
- 5.2.20 When certification is required (see Section 13), and and site h.a.)
- 5.2.21 Special marking requirements (see Section 14),
- 5.2.22 Special packaging or package marking requirements (see Section 15),
- 5.2.23 When ISO 9001 quality assurance system is not required (see 16.1), and
- 5.2.24 Special warranty requirements (see 16.2).

6. Materials and Manufacture

6.1 Sensing Elements—The materials for the sensing element and wetted parts shall be selected for long-term compatibility (see 8.1) with the process medium (see 4.4).

7. Physical Properties

7.1 Enclosure—If case sealing is required, the mechanism, materials, and process shall be described. The same should apply to the electrical connector. The long-term resistance to common process media should be stated. Resistance to cleaning solvents should likewise be stated. Unique or special enclosure requirements shall be specified in the acquisition requirements (see 5.2).

7.2 Transducer Mounting—Transducers are commonly mounted directly by their pressure connections or through the use of brackets or similar hardware. Mounting force or torque shall be specified if it tends to affect transducer performance. Mounting error shall be specified in terms of percent of full-scale output or within the static error band under specified conditions of mounting force or torque.

7.3 External Configuration—The outline drawing shall show the configuration with dimensions in SI units (inch-pound units). The outline drawing shall include limiting dimensions for pressure and electrical connections if they are not specified. The outline drawing shall indicate the mounting method with hole size, center location, and other pertinent dimensions. Where threaded holes are used, thread specifications shall be provided.

7.4 Standard Electrical Connection-An electrical interface connector receptacle and mating plug shall be provided with each transducer unless otherwise specified in the contract (see 5.1). Optional possible electrical interface connections include pigtails and terminal boards.

7.5 Pressure Connections—Pressure connections commonly consist of pipe thread, hose tube fittings, O-ring union, O-ring union face seal, and others.

7.6 Damping—The use of a media for damping in transducers shall be specified including the type, composition, and compatibility with transducer components and materials.

7.7 Size and Weight—The purchaser may have intended applications in which size and weight are limited. Size and weight restrictions shall be specified in the ordering information (see 5.2).

8. Performance Requirements

8.1 *Service Life*—The purchaser may have a minimum specified service life requirement that may be critical. Critical service life requirements shall be specified in the ordering information (see 5.2).

8.2 *Transducer Performance*—Performance tolerances are usually specified in percent of transducer output span. Critical performance requirements shall be specified in the ordering information (see 5.2). The following performance characteristics and environmental exposures may or may not be important to each purchaser's intended application: static error band, repeatability, hysteresis, sensitivity factor, ripple, warm-up time, steady-state supply voltage and frequency (ac), steady-state supply voltage (dc), response, transient supply voltage and frequency (ac), transient supply voltage (dc), temperature, humidity, overpressure, line pressure (differential only), salt spray, pressure cycling, insulation resistance, vibration, shock, burst pressure, output, enclosure, electromagnetic interference (EMI), common mode pressure (differential only), pressure rating (differential only), and power system harmonic distortion.

9. Workmanship, Finish, and Appearance

9.1 *Finish and Appearance*—Any special surface finish and appearance requirements shall be specified in the ordering information (see 5.2).

9.2 Transducer Cleaning—Any special cleaning requirements shall be specified in the ordering information (see 5.2).

10. Number of Tests and Retests

10.1 *Test Specimen*—The number of test specimens to be subjected to first-article tests shall be specified and should depend on the transducer design. As guidance, if each range is covered by a separate and distinct design, a test specimen for each range should require testing. In instances in which a singular design series may cover multiple ranges and types, a minimum of three test specimens should be tested provided the electrical, optical, and mechanical similarities are approved by the purchaser. It is suggested that three units, one unit each representing the low, medium, and high ranges, be tested, regardless of design similarity.

10.1.1 Low Range—Less than 700 kPa (less than 100 lb/in.²).

- 10.1.2 Medium Range-700 kPa to less than 7 MPa (100 to less than 1000 lb/in.²).
- 10.1.3 *High Range*—7 MPa and greater (1000 lb/in.² and greater).

11. Test Methods

11.1 *Test Data*—All test data shall remain on file at the manufacturer's facility for review by the purchaser upon request. It is recommended that test data be retained in the manufacturer's files for at least three years, or a period of time acceptable to the purchaser and the manufacturer. alog/standards/sist/48218ac-5ca8-42319d41135276343e0dastm-2070-002017

12. Inspection

12.1 *Classification of Inspections*—The inspection requirements specified herein are classified as follows:

- 12.1.1 First-article tests (see 12.2).
- 12.1.2 Conformance tests (see 12.3).

12.2 *First-Article Tests*—First-article test requirements shall be specified, where applicable. First-article test methods should be identified for each design and performance characteristic specified. Test report documentation requirements should also be specified.

12.3 *Conformance Tests*—Conformance testing shall be specified when applicable. Conformance testing shall be conducted on all units manufactured for delivery unless otherwise specified in the contract.

13. Certification

13.1 When specified in the acquisition requirements (see 5.2), the purchaser shall be furnished certification that samples representing each lot have been either tested or inspected as directed in this specification and the requirements have been met.


14. Product Marking

14.1 The purchaser specified product marking shall be listed in the acquisition requirements (see 5.2). The minimum data to be clearly marked on each transducer shall include the following:

14.1.1 Manufacturer's name,

- 14.1.2 Manufacturer's part number,
- 14.1.3 Serial number or lot number,
- 14.1.4 Date of manufacture,

14.1.5 Range,



14.1.6 Excitation voltage, and

14.1.7 Pressure rating (differential pressure transducers only).

14.2 For differential pressure transducers, the high- and low-pressure connections shall be clearly marked on the transducer body adjacent to the connections.

15. Packaging and Package Marking

15.1 Packaging of Product for Delivery-The product should be packaged for shipment in accordance with Practice D3951.

15.2 Any special packaging or package marking requirements for shipment or storage shall be identified in the ordering information (see 5.2).

16. Quality Assurance

16.1 *Quality System*—A quality assurance system in accordance with ISO 9001 shall be maintained to control the quality of the product being supplied effectively, unless otherwise specified in the acquisition requirements (see 5.2).

16.2 Responsibility for Warranty-Unless otherwise specified, the manufacturer is responsible for the following:

16.2.1 All materials used to produce a unit and

16.2.2 Workmanship to produce the unit.

16.3 Special warranty requirements shall be specified in the acquisition requirements (see 5.2).

17. Keywords

17.1 differential pressure transmitter; fiber-optic pressure transducer; miniature; optoelectronics module; pressure and differential pressure transducers; pressure transmitter; sensing element; sensor head; transduction element

SUPPLEMENTARY REQUIREMENTS

The following supplementary requirement, established for U.S. naval shipboard application, shall apply when specified in the contract or purchase order. When there is conflict between this specification (Specification F2070) and this supplementary requirement, this supplementary requirement shall take precedence. This document supersedes MIL-T-24742, *Transducer, Pressure and Differential Pressure, Miniature (Electrical)*, for new ship construction.

<u>5TM F2070-00(2017)</u>

https://standards.iteh.ai/catalog/standards/sist/482ff8ac-5ca8-423f-9d41-f35276343e0d/astm-f2070-002017

S1. TRANSDUCERS, PRESSURE AND DIFFERENTIAL PRESSURE, MINIATURE (ELECTRICAL)

S1.1 Scope

S1.1.1 This supplement covers the requirements for miniature pressure and differential pressure transducers designed to meet the requirements for use onboard naval ships.

S1.1.2 The values stated in SI units are to be regarded as the standard. Inch-pound units standard. The values given in parentheses are mathematical conversions to inch-pound units that are provided for information only. only and are not considered standard. Where information is to be specified, it shall be stated in SI units.

S1.2 Referenced Documents


S1.2.1 ISO Standard: Standards:⁴

6149-1 Connections for Fluid Power and General Use—Ports and Stud Ends with ISO 261 Threads and O-Ring Sealing—Part 1: Ports with O-Ring Seal in Truncated Housing

S1.2.2 NEMA Standard: Standards: 5

250 Enclosures for Electrical Equipment (1000 Volts Maximum)

⁵ Available from National Electrical Manufacturers Association (NEMA), 1300 N. 17th St., Suite 1847, Rosslyn, VA 22209.900, Arlington, VA 22209, http:// www.nema.org.



S1.2.3 Military Standards:⁶

MIL-S-901 Shock Tests, H.I. (High-Impact); Shipboard Machinery, Equipment and Systems, Requirements for MIL-STD-167-1 Mechanical Vibrations of Shipboard Equipment (Type I—Environmental and Type II—Internally Excited) MIL-STD-461 Electromagnetic Interference Characteristics of Subsystems and Equipment, Requirements for the Control of MIL-STD-1399, Section 300 Interface Standard for Shipboard Systems, Electric Power, Alternating Current MS3452 Connector, Receptacle, Electric, Box Mounting, Rear Release, Crimp Contact, AN Type

MS3456 Connector, Plug, Electrical, Rear Release, Crimp Contact, AN type

S1.3 Terminology

S1.3.1 Terminology is consistent with that of Section 3 and the referenced documents.

S1.4 Designation

S1.4.1 *Designation*—For this specification pressure transducers, designations shall be assigned in accordance with S1.5.1 and listed in the following below:

iTeh Standards (https://standards.iteh.ai) Document Preview

ASTM F2070-00(2017)

https://standards.iteh.ai/catalog/standards/sist/482ff8ac-5ca8-423f-9d41-f35276343e0d/astm-f2070-002017

⁶ Available from U.S. Government Standardization Documents Order Desk, DLA Document Services, Building 4/D, 700 Robbins Ave., Philadelphia, PA 19111. 19111-5094, http://quicksearch.dla.mil.

Example: F25XMS1-D-F-5-DC-2-N-M-100D

	Example: F25XMS1-D-F-5-DC-2-N-M-100D								
	Specification	Ð	F	5	ĐC	2	N	M	100D
	F25XMS1	Туре	Application	Press Rating	Power Supply	Output	Press Conn	Mounting	Range
		\$1.4.2	S1.4.3	S1.4.4	\$1.4.5	S1.4.6	\$1.4.7	S1.4.8	\$1.4.9
	Specification	D	F	5	DC	_2	<u>N</u>	M	100D
	F25XMS1	Туре	Application	Press Rating	Power Supply	Output	Press Conn	Mounting	Range
I		<u>S1.4.2</u>	<u>S1.4.3</u>	<u>S1.4.4</u>	<u>S1.4.5</u>	<u>S1.4.6</u>	<u>S1.4.7</u>	<u>S1.4.8</u>	<u>S1.4.9</u>

S1.4.2 Types—The following designators have been established for the various types of transducers:

D-Pressure, differential

P—Pressure (gage, absolute and sealed)

V—Pressure, vacuum

C-Pressure, compound

\$1.4.3 Application—The following application designations have been established for the corresponding process media:

F-Freshwater, oil, condensate, steam, nitrogen, and other inert gases

S—Seawater

G-Flue gas and ammonia

X—Oxygen

S1.4.4 *Pressure Rating*—The pressure rating shall be indicated by the designator for its numerical value for Type D transducers ("X" for Type P, V, and C transducers) and shall be limited to the following:

Designator	Rating, kPaG	Inch-Pound, psig
1	100	15
2		150
3	2 000	300
4	4 000	600
5	10 000	1500
6		3000
7	40 000	6000

S1.4.5 *Power Supply*—Transducers shall operate with either ac or dc input power, but not both. Designators shall be as follows: S1.4.5.1 dc—Direct-current supply. <u>ASTM F2070-00(2017)</u>

S1.4.5.2 ac-Alternating-current supply.lards/sist/482ff8ac-5ca8-423f-9d41-f35276343e0d/astm-f2070-002017

S1.4.6 *Output*—The dc electrical signal output of the transducer shall be designated by the following designators:

2-4-20 mA

3—0-5 V

4—0-12 V

5—0-3 mV

6-0-200 µV

S1.4.7 Pressure Connection—Transducer pressure sensing connection shall be as follows:

N—M12 × 1.5 (7/16-20 UNF-2B) (see S1.7.5)

X—¹/₄ nps, 155-mm (6-in.) long pipe nipple (see S1.7.5)

Z—Other

S1.4.8 Transducer Mounting—The transducer mounting method shall be designated as follows:

P-Pressure port connection

M-Mounting plate

S1.4.9 *Range*—The pressure range of the transducer shall be designated by two parts. The first part shall be the designator for the upper range value. The second part shall be the designator for the upper range unit of measure (see S1.4.9.1). The transducer pressure ranges shall be in accordance with Table S1.1.

S1.4.9.1 Units—The units shall be designated by the corresponding letter designator and are limited to the following:

TABLE S1.1 Range

Туре D			Туре Р			Туре С		Type V			
					SI U						
Differential Pressure Differential Pressure V						Compound Ranges,		Vacuum Range,			
Ranges, kPaD Column Ranges, kPaWD			kPaA or kPaS ^A		kPaW		kPaV/kPaG		kPaV		
Range	Designator	Range	Designator	Range	Designator	Range	Designator	Range	Designator	Range	Designato
0-100	100	0-2.5	2	0-100	100	0-2.5	2	100/150	150	0-100	100
0-200	200	0-15	15	0-200	200	0-15	15	100/300	300		
0-400	400	0-40	40	0-350	350	0-40	40	100/900	900		
0-700	700	0-75	75	0-400	400	0-75	75	100/1500	1500		
0-1400	1400			0-700	700			100/2400	2400		
0-2800	2800			0-850	850			100/4000	4000		
0-4000	4K			0-1 400	1400						
				0-2 000	2K						
				0-4 000	4K						
				0-6 000	6K						
				0-7 000	7K						
				0-10 000	10K						
				0-20 000	20K						
				0-40 000	40K						
				0-70 000	70K						
					Inch-Pou						
	al Pressure		Pressure Water	Pressure F	langes, psig,		umn Ranges,		d Ranges,		n Range,
	es, psid		Ranges, WCD		or psis ^A		VC)-psig		Hg
Range	Designator	Range	Designator	Range	Designator	Range	Designator	Range	Designator	Range	Designato
		0		0 1 5	100	0-10	2	30-0-15	150	0-30	100
0-15	100	0-10	2	0-15							
0-15 0-30	100 200	0-60	15	0-30	200	0-60	15	30-0-30	300		
0-15 0-30 0-60	100 200 400	0-60 0-150	15 40	0-30 0-50	350	0-60 0-150	15 40	30-0-30 30-0-100	900		
0-15 0-30 0-60 0-100	100 200 400 700	0-60	15	0-30 0-50 0-60	350 400	0-60	15	30-0-30 30-0-100 30-0-150	900 1500		
0-15 0-30 0-60 0-100 0-200	100 200 400 700 1400	0-60 0-150	15 40	0-30 0-50 0-60 0-100	350 400 700	0-60 0-150	15 40	30-0-30 30-0-100 30-0-150 30-0-300	900 1500 2400		
0-15 0-30 0-60 0-100	100 200 400 700	0-60 0-150	15 40	0-30 0-50 0-60 0-100 0-125	350 400 700 850	0-60 0-150	15 40	30-0-30 30-0-100 30-0-150	900 1500		
0-15 0-30 0-60 0-100 0-200	100 200 400 700 1400	0-60 0-150	15 40	0-30 0-50 0-60 0-100 0-125 0-200	350 400 700 850 1400	0-60 0-150	15 40	30-0-30 30-0-100 30-0-150 30-0-300	900 1500 2400		
0-15 0-30 0-60 0-100 0-200 0-400	100 200 400 700 1400 2800	0-60 0-150	15 40	0-30 0-50 0-60 0-100 0-125	350 400 700 850 1400 2K	0-60 0-150	15 40	30-0-30 30-0-100 30-0-150 30-0-300	900 1500 2400		
0-15 0-30 0-60 0-100 0-200 0-400	100 200 400 700 1400 2800	0-60 0-150	15 40	0-30 0-50 0-60 0-100 0-125 0-200 0-300 0-600	350 400 700 850 1400 2K 4K	0-60 0-150	15 40	30-0-30 30-0-100 30-0-150 30-0-300	900 1500 2400		
0-15 0-30 0-60 0-100 0-200 0-400	100 200 400 700 1400 2800	0-60 0-150	15 40	0-30 0-50 0-60 0-100 0-125 0-200 0-300 0-600 0-900	350 400 700 850 1400 2K 4K 6K	0-60 0-150	15 40	30-0-30 30-0-100 30-0-150 30-0-300	900 1500 2400		
0-15 0-30 0-60 0-100 0-200 0-400	100 200 400 700 1400 2800	0-60 0-150	15 40	0-30 0-50 0-60 0-100 0-125 0-200 0-300 0-300 0-900 0-1000	350 400 700 850 1400 2K 4K 6K 7K	0-60 0-150	15 40	30-0-30 30-0-100 30-0-150 30-0-300	900 1500 2400		
0-15 0-30 0-60 0-100 0-200 0-400	100 200 400 700 1400 2800	0-60 0-150	15 40	0-30 0-50 0-60 0-100 0-125 0-200 0-300 0-600 0-900 0-1 000 0-1 500	350 400 700 850 1400 2K 4K 6K 7K 10K	0-60 0-150	15 40	30-0-30 30-0-100 30-0-150 30-0-300	900 1500 2400		
0-15 0-30 0-60 0-100 0-200 0-400	100 200 400 700 1400 2800	0-60 0-150	15 40	0-30 0-50 0-60 0-100 0-125 0-200 0-300 0-300 0-900 0-1000	350 400 700 850 1400 2K 4K 6K 7K	0-60 0-150	15 40	30-0-30 30-0-100 30-0-150 30-0-300	900 1500 2400		
0-15 0-30 0-60 0-100 0-200 0-400	100 200 400 700 1400 2800	0-60 0-150	15 40	0-30 0-50 0-60 0-100 0-125 0-200 0-300 0-600 0-900 0-1 000 0-1 500	350 400 700 850 1400 2K 4K 6K 7K 10K	0-60 0-150	15 40	30-0-30 30-0-100 30-0-150 30-0-300 30-0-600	900 1500 2400		

^A For upper range values of 7000 kPa (1000 lb/in.²) and above.

ASTM F2070-00(2017) https://standards.iteh.ai/catalog/standards/studies/f8ac-5ca8-423f-9d41-f35276345CVPastmet2070-002017

V	kPaV—kiloPascals, vacuum	Hg—inches of mercury vacuum
A	kPaA—kiloPascals, absolute	psia—pounds per square inch, absolute
D	kPaD—kiloPascals, differential	psid—pounds per square inch, differential
G	kPaG—kiloPascals, gage	psig—pounds per square inch, gage
S	kPaS—kiloPascals, sealed at 101.4 kPaA	psis—pounds per square inch, sealed at 14.7 psia
W	kPaW—kiloPascals, water column	WC—inches of water column
Ν	KPaWD—kiloPascals, water column, differential	WCD—inches of water column, differential

S1.5 Ordering Information

\$1.5.1 The purchaser shall provide the manufacturer with all of the pertinent application data in accordance with \$1.5.2. If special application operating conditions exist that are not in the acquisition requirements, they shall also be described.

S1.5.2 Acquisition Requirements—Acquisition documents shall specify the following:

- S1.5.2.1 Title, number, and date of this specification.
- S1.5.2.2 Part designation.
- S1.5.2.3 National Stock Number (NSN), if available.
- S1.5.2.4 Mounting method, if other than specified herein.
- S1.5.2.5 Type of pressure connection, if other than specified herein.
- S1.5.2.6 Type of electrical connection, if other than specified herein.
- S1.5.2.7 When the electrical connection mating plug is not to be provided.
- S1.5.2.8 Quantity of transducers required.
- \$1.5.2.9 If deviation requests are required when departing from material guidance.
- S1.5.2.10 When first-article tests are required.
- S1.5.2.11 Special product marking requirements.
- S1.5.2.12 Special packaging or package marking requirements.
- S1.5.2.13 When ISO 9001 quality assurance system is not required.
- S1.5.2.14 Special warranty requirements.

\$1.5.3 First-Article Tests—When first-article testing is required, the purchaser should provide specific guidance to offerors whether the item(s) should be a preproduction sample, a first-article sample, a first production item, a sample selected from the first production items, or a standard production item from the manufacturer's current inventory. The number of items to be tested in accordance with \$1.12.4 should be specified. The purchaser should include specific instructions in acquisition documents regarding arrangements for tests, approval of first-article test results and time period for approval, and disposition of first articles. Invitations for bids should provide that the purchaser reserves the right to waive the requirement for samples for first-article testing to those manufacturers offering a product that has been previously acquired or tested by the purchaser; and that manufacturers offering such products, who wish to rely on such production or test, must furnish evidence with the bid that prior purchaser approval is presently appropriate for the pending contract. The manufacture of items before purchaser approval should be specified as the responsibility of the manufacturer.

S1.6 Materials

\$1.6.1 Sensing Elements—The materials for the sensing element and wetted parts shall be selected for long-term compatibility (see \$1.8.1) with the process medium (see \$1.4.3). Table \$1.2 is provided for guidance as acceptable material and process medium compatibility. Dissimilar metals shall not be used in contact with each other unless suitably finished to prevent electrolytic corrosion. When departing from this guidance, the manufacturer shall provide evidence of material compatibility to the procuring activity, unless specified otherwise (see S1.5.1).


S1.7 Physical Properties

S1.7.1 Enclosure—The transducer body and pressure cavity shall be environmentally sealed unless otherwise specified. The transducer enclosure shall be Type 4 in accordance with NEMA Standard 250.

S1.7.2 Transducer Mounting—The transducer shall have a mounting plate as shown on Fig. S1.1. If required in a specific application and with prior approval of the purchaser, the transducer may be mounted by its pressure piping connection. For Type D transducers, the high-pressure port shall be used. If the transducer is mounted by its pressure connection, the mounting plate shall not be required (see \$1.5.2). If the transducer is mounted by its pressure port connection and the mounting plate is provided, mounting holes shall not be required.

TABLE S1.2 Material Versus Application						
Sensing Element and Wetted Parts	Process Medium					
		Application Designation S				
CRES 304L, 316L, 321 & 347	х		Х			
CRES 15-5 PH, 17-4 PH, and 17-7 PH	х					
Monel and K-Monel	Х	Х		Х		
Inconel 600 and 750	Х	Х				
Inconel 625 and 718	Х	Х				
Hastelloy C276	Х	Х	Х			
Titanium CP and 6A1-4V	Х	Х				
CuNi 70/30	Х	Х		Х		
Ni Span	Х					
Tantalum	Х	Х				
Carpenter A286			Х	Х		

TABLE S1.2 Material	Versus	Application
---------------------	--------	-------------

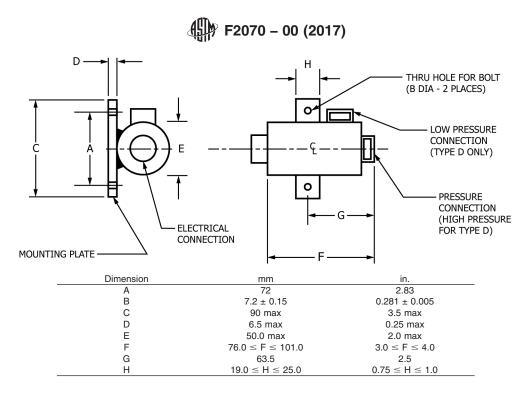

NOTE 1—Transducer housing (body) cross section is shown as circular. Any alternate cross section not exceeding 50 mm (2 in.) in width and 50 mm (2 in.) in height is acceptable.

NOTE 2-Dimension tolerance is plus or minus 1.25 mm (0.05 in.), unless otherwise specified.

NOTE 3—The pressure connection(s) shall be generally located as shown.

FIG. S1.1 External Configuration

S1.7.3 *External Configuration*—The transducer shall have an external configuration within the boundaries established by Fig. S1.1.

S1.7.4 *Electrical Connector*—An electrical interface connector receptacle and mating plug shall be provided with each transducer unless otherwise specified. The electrical connector shall be a standard threaded coupling receptacle, AN type, MS3452W/14S-5P, or equivalent, for dc-power input, or AN type, MS3452W/14S-5PX, or equivalent, for ac-power input. The mating plug shall be a MS3456W/14S-5S, or equivalent, for dc-power input, or MS3456W/14S-5SX, or equivalent, for ac-power input.

S1.7.4.1 *dc-Power Input—Output* 2—The receptacle shall be wired to provide the performance described herein. Receptacle Pin A shall be +28-Vdc power input, Pin B shall be -28-Vdc power input, and Pin C shall be case ground. Receptacle Pins A and B shall also serve as the 4- to 20-mA dc signal output.

S1.7.4.2 *dc Power Input—Output 3, 4, 5, 6*—The receptacle shall be wired to provide the performance described herein. Receptacle Pin A shall be +28-Vdc power input, Pin B shall be –28-Vdc power input, Pin C shall be case ground, Pin D shall be positive dc voltage signal output, and Pin E shall be negative dc voltage signal output.

S1.7.4.3 *ac Power Input—Output 2*—The receptacle shall be wired to provide the performance described herein. Receptacle Pins A and B shall be 115-Vac power input, Pin C shall be case ground, Pin D shall be +4- to 20-mA dc-signal output, and Pin E shall be -4- to 20-mA dc signal output.

S1.7.4.4 *ac Power Input—Output 3, 4, 5, 6*—The receptacle shall be wired to provide the performance described herein. Receptacle Pins A and B shall be 115-Vac power input, Pin C shall be case ground, Pin D shall be positive dc-voltage signal output, and Pin E shall be negative dc voltage signal output.

S1.7.5 *Pressure Connections*—Unless otherwise specified, transducer pressure-sensing connections for all services shall be M12 × 1.5 (7/16-20 UNF-2B) tube connection in accordance with ISO 6149-1. When pressure connection Type X is specified, as commonly used on submarine oxygen replenishment systems, the transducer sensing connections shall be a nickel-copper pipe nipple $\frac{1}{4}$ nominal pipe size (nps) with 3.1-mm (0.12-in.) minimum wall thickness, 155 mm (6 in.) long, welded to the socket (see S1.5.2). For Type D transducers, the high-pressure connection shall be on the end and the low-pressure connection shall be on the side (see Fig. S1.1).

S1.7.6 Welding—For Application X, all pressure boundary joints shall be welded.

S1.7.7 Lubrication—The transducer shall operate without lubrication of moving parts after assembly.

- S1.7.8 Damping—The use of a media for damping in transducers shall be cited on the equipment drawing.
- S1.7.9 Weight—The weight of a transducer shall not exceed 510 g (18 oz).