



Designation: D1082 – 17

Standard Test Method for Dissipation Factor and Permittivity (Dielectric Constant) of Mica¹

This standard is issued under the fixed designation D1082; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope*

1.1 This test method covers the determination of the dissipation factor and the relative permittivity of natural block mica having thicknesses between 0.007 and 0.030 in. (0.18 and 0.77 mm) and mica films or capacitor splits between 0.0008 and 0.004 in. (0.02 and 0.10 mm) in thickness.

1.2 The values stated in inch-pound units are to be regarded as the standard. The values in parentheses are for information purposes only.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.* A specific warning statement is given in Section 7 and 6.1.1.

NOTE 1—Procedures for the measurement of dissipation factor and permittivity are given in IEC Publication 60371-2, but the details of the procedure are somewhat different from those specified in this test method.

1.4 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 ASTM Standards:²

- D150 Test Methods for AC Loss Characteristics and Permittivity (Dielectric Constant) of Solid Electrical Insulation
- D374 Test Methods for Thickness of Solid Electrical Insulation (Metric) D0374_D0374M

¹ This test method is under the jurisdiction of ASTM Committee D09 on Electrical and Electronic Insulating Materials and is the direct responsibility of Subcommittee D09.01 on Electrical Insulating Products.

Current edition approved Nov. 1, 2017. Published December 2017. Originally approved in 1949. Last previous edition approved in 2011 as D1082 – 00 (2011). DOI: 10.1520/D1082-17.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

D748 Specification for Natural Block Mica and Mica Films Suitable for Use in Fixed Mica-Dielectric Capacitors

2.2 IEC Publication:

Publication 60371-2 Specification for insulating materials based on mica—Part 2: Methods of test³

3. Summary of Test Method

3.1 Any of the techniques and apparatus set forth in Test Methods D150 are suitable for measuring dissipation factor and relative permittivity of block mica or film. Select an appropriate electrode system from those given in Section 5.

3.2 If a relative order of magnitude of dissipation factor is desired, the use of Method A in the Appendix of Specification D748 is satisfactory.

4. Significance and Use

4.1 The dissipation factor of natural muscovite mica, as determined by this test method, is of practical importance as a measure of the electrical energy lost as heat in the mica serving as the dielectric substance of capacitors, or in other applications in which the electric field is applied perpendicular to the plane of cleavage. The dissipation factor is particularly important in applications using mica at radio frequencies and in some less extensive audio frequency applications. This test method is suitable for specification acceptance and dielectric-loss control tests (see the Significance and Use of Test Methods D150).

4.2 *Relative Permittivity (Dielectric Constant)*—The permittivity of natural muscovite mica is a measure of its relative ability to store electrostatic energy. Since the relative permittivity perpendicular to the cleavage plane is fairly uniform, regardless of origin, its practical significance is mainly for identification purposes, special uses, research, and design. If a loss index is desired, the value of the permittivity must be known (see the Significance and Use of Test Methods D150).

5. Apparatus

5.1 For a general description of apparatus suitable for measuring dissipation factor and relative permittivity, refer to Test Methods D150.

³ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036.

*A Summary of Changes section appears at the end of this standard

5.2 Select a suitable electrode arrangement from the following:

5.2.1 *Steel Electrodes*—Three electrodes made of stainless steel or nickel-plated tool steel will be required. The electrodes shall be cylindrical in shape and of a diameter sufficient to provide the minimum specified capacitance (Note 2). The upper and lower electrodes shall have a minimum axial length of 1/2 in. (12.7 mm) and the center electrode shall have a maximum length of 1/4 in. (6.35 mm). A low-resistance contact and conductor to the electrode is essential for dissipation factor measurements in the order of 0.0001. The upper and lower electrodes shall be electrically connected together, thus forming a two-terminal capacitor, with the center electrode serving as the active or measuring terminal. The surfaces of the electrodes adjacent to the specimen shall be ground and polished optically flat, and shall be parallel to each other. The upper electrode shall be provided with a recess for a steel ball, so that the applied pressure will be uniformly distributed. The electrodes shall be carefully and accurately aligned without scratching the surface of the mica specimen. It is recommended that a slotted V-shaped jig be provided to aid with the aligning of the electrodes.

NOTE 2—Steel electrodes having diameters of 3/4, 1, 1 1/4, and 1 1/2 in. (19, 25, 32, and 38 mm) have been found satisfactory for practical thicknesses of mica specimens.

5.2.2 *Mercury Electrodes*—Three hollow, stainless steel or nickel-plated cold-rolled steel electrodes mounted with the axis horizontal so that the test specimens are in a vertical plane, will be required as shown in Fig. 1. The electrode assembly shall be cylindrical in shape and of the same outside diameter, which shall be large enough to provide the minimum specified capacitance (Note 3). Two adjustable electrodes having axial lengths of approximately 3/4 in. (19 mm), provided with suitable cavities, shall be mounted on screws in a solid stainless steel or nickel-plated cold-rolled steel rectangular yoke. A center, or fixed, electrode consisting of a hollow ring approximately 3/8 in. (9.5 mm) in length shall be mounted at the center of the steel yoke on a support of insulating material such as polystyrene, hard rubber, low-loss ceramic, or quartz. All electrodes shall taper from the inside to rather sharp edges approximately 1/64 in. (0.4 mm) in width.

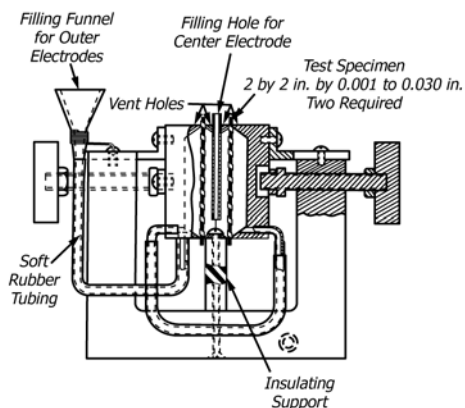


FIG. 1 Mercury Electrode Test Assembly

5.2.2.1 The two outer electrodes shall be provided with a rubber tube attached to 1/8-in. (3.2-mm) steel tubes located at the bottom of each electrode. Small vent holes shall be provided in the top of the outer electrodes to permit the escape of entrapped air as the mercury rises. The center electrode shall be filled through a 1/8-in. steel tube projecting approximately 1/8 in. above the top of the electrode and extending three fourths of the way down inside the steel ring. Vent holes shall be provided on either side of the projecting steel tube to permit entrapped air to escape as the mercury rises. With the test specimens clamped in position, the electrodes shall be in good alignment. As in the case of the flat, steel electrodes, a two-terminal capacitor is formed with the center electrode serving as the active or measuring terminal with the outer electrodes that are connected together by the steel yoke at the ground.

NOTE 3—Mercury electrodes having diameters of 1 3/4 in. (44.5 mm) have been found satisfactory for mica specimens 2 by 2 in. by 0.001 to 0.030 in. (51 by 51 mm by 0.025 to 0.76 mm).

NOTE 4—Conducting paint electrodes can be substituted for mercury electrodes.

5.2.3 *Lead-Foil Electrodes*—The use of lead-foil electrodes 0.0005 in. (0.013 mm) in thickness and 2.0 in. (51 mm) in diameter is satisfactory for block mica 0.015 to 0.030 in. (0.38 to 0.76 mm) in thickness. (See also metal-foil electrodes described in the Section of Test Methods D150 under Electrode Systems).

5.3 The apparatus for the rapid, direct-reading method is set forth in Appendix of Specification D748. This technique is for use only where classification of relative magnitude of dissipation factor (or its reciprocal Q value) of block mica or films is desired.

5.4 Thickness-measuring apparatus shall conform to the requirements set forth in Test Method A of Test Methods D374 which describes a machinist's micrometer caliper with a ratchet or friction thimble.

6. Specimen Preparation and Conditioning

6.1 The dielectric properties of mica are affected by temperature, humidity, pressure, etc. Therefore, preparation and conditioning of the specimen shall be made in the following manner:

6.1.1 With the exception of the specimens used in 5.4, thoroughly and carefully clean the surfaces of the specimen with a camel's-hair brush dipped in petroleum ether or vapor degrease using trichloroethylene. Subsequent to the cleaning, exercise care not to contaminate the surfaces in handling. (Warning—Petroleum ether and trichloroethylene are hazardous. Use adequately ventilated work areas and observe all procedures for the safe handling of these liquids. Keep away from open flames.)

6.1.2 After cleaning, place each specimen in an air oven maintained at 105 to 110°C, for a period of 1 h. Upon removal from the oven, immediately store the specimen in a desiccator until ready for the test.

6.2 Prepare two similar test specimens of approximately equal and uniform thickness for each measurement when using steel or mercury electrodes (see Section 5).