



Standard Specification for Indicators, Sight, Liquid Level, Direct and Indirect Reading, Tubular Glass/Plastic¹

This standard is issued under the fixed designation F2045; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This standard has been approved for use by agencies of the U.S. Department of Defense.

^{ε1} NOTE—A key was editorially added to Fig. 1 in January 2018.

1. Scope

1.1 This specification covers the requirements for direct and indirect reading sight liquid level indicators for general applications. General applications for indirect reading sight glasses are water and fuel service at working pressures 2.07 MPa (300 lb/in.²) and below, temperatures of 149°C (300°F) and below. General applications for direct reading sight glasses are applications in which the temperature does not exceed 66°C (150°F).

1.2 Direct reading sight glass indicators may consist of glass or plastic tubes with fittings including shutoff valves. Glass tubes may be used for low shock direct reading sight glass indicators in which the fluid is not compatible with plastic.

1.3 Indirect reading indicators may consist of a sealed chamber with a magnetic float or flag indicator.

1.4 Special requirements for naval shipboard applications are included in the supplement to this standard.

1.5 The values stated in SI units are to be regarded as standard. The values given in parentheses are mathematical conversions to inch-pound units that are provided for information only and are not considered standard.

1.6 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

¹ This specification is under the jurisdiction of ASTM Committee F25 on Ships and Marine Technology and is the direct responsibility of Subcommittee F25.10 on Electrical.

Current edition approved Jan. 1, 2018. Published January 2018. Originally approved in 2000. Last previous edition approved in 2011 as F2045 – 00 (2011). DOI: 10.1520/F2045-00R18E01.

2. Referenced Documents

2.1 *ASTM Standards*:²

D3951 Practice for Commercial Packaging

2.2 *ANSI Standards*:³

B16.5 Pipe Flanges and Flanged Fittings (DoD adopted)

3. Terminology

3.1 *Definitions*:

3.1.1 *SI (Le Systeme International d'Unites) Units*—units of measurement recognized by the CIPM (Comite' International des Poids et Mesures).

4. Design Classification


4.1 *Types*—Indicator designs are classified as either direct reading or indirect reading. Both types are depicted in Fig. 1, complete with dimensions that facilitate ordering.

4.2 *Special Considerations*—Special considerations that may affect selection and installation are listed below. This is not to be construed as a complete listing.

- (1) Type of indicator,
- (2) Manual or automatic shutoff valves,
- (3) Indication length of liquid level range,
- (4) Method of connection,
- (5) Location of indicator relative to vibrating equipment,
- (6) Protection of the instrumentation,
- (7) Application of each indicator,
- (8) Cleaning procedure or reference to the cleaning procedure being used, and

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, http://www.ansi.org.

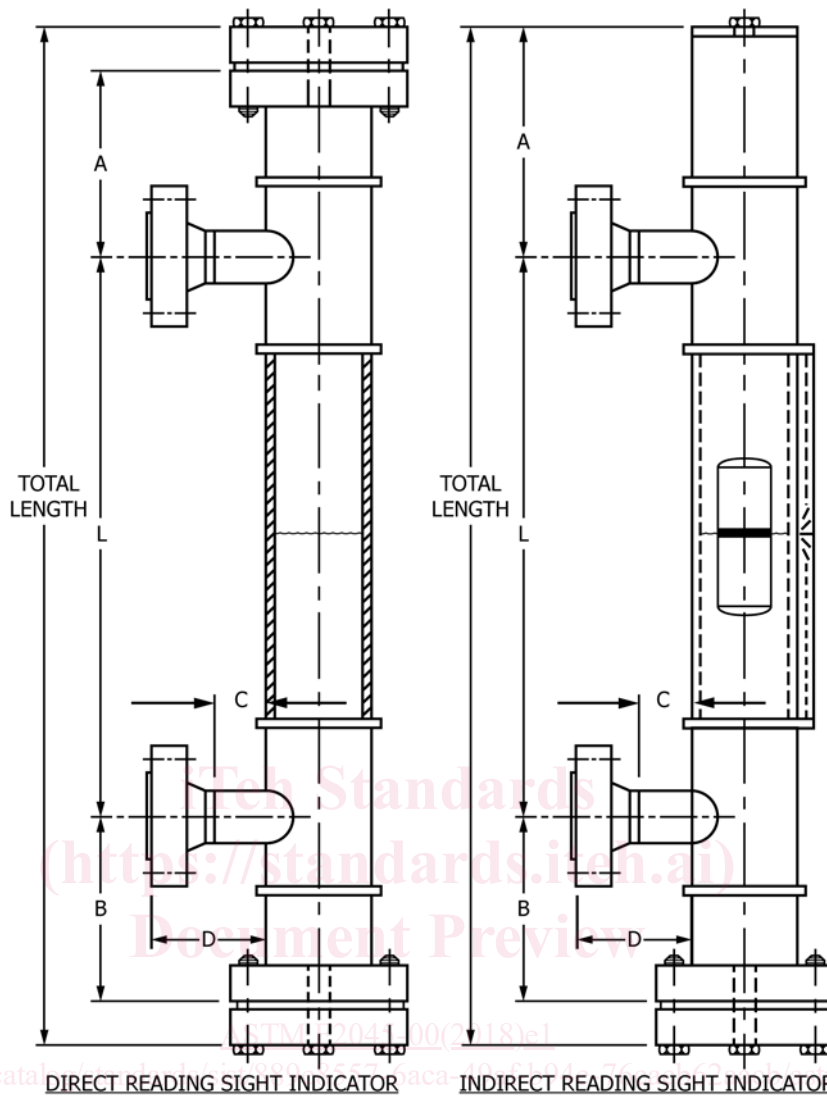

Dimensions (mm)

A	Distance between center of top attachment flange face and top of indicator tube
B	Distance between center of bottom attachment flange face and bottom of indicator tube
C	Length of piping between outer tube wall and connection to tank attachment flange
D	Distance between outer tube wall and outer edge of tank attachment flange
L	Distance between center of attachment flange faces

FIG. 1 Indicator Design Types

(9) Selection of indicator for compatibility with materials, temperature, pressure, ambient environment, and with the parameter being measured.

5. Ordering Information

5.1 The buyer shall provide the manufacturer with all of the pertinent application data outlined in the acquisition requirements.

5.2 *Acquisition Requirements*—Acquisition documents shall specify the following:

- (1) Title, number, and date of this specification;
- (2) Type and quantity of indicators required;
- (3) Manufacturer’s part number;
- (4) When qualification testing is required;

- (5) Final disposition of qualification test samples;
- (6) Environmental requirements;
- (7) Operating media;
- (8) Viscosity and specific gravity of fluid for indirect indicators;
- (9) Materials;
- (10) Indication length;
- (11) Size and type of connections;
- (12) Shutoff valve requirements;
- (13) Cleaning requirements;
- (14) When certification is required;
- (15) Marking requirements;
- (16) Unique packaging requirements; and
- (17) Unique preservation requirements.

6. Materials and Manufacture

6.1 *Materials*—The materials for all wetted parts shall be selected for long-term compatibility with the process medium and ambient conditions.

6.2 *Material Inspection*—The manufacturer shall be responsible for ensuring that materials used are manufactured, examined, and tested in accordance with the specifications and standards as applicable.

6.3 *Gaskets and O-Rings*—Gaskets and O-rings shall be fabricated of materials suitable to the operating pressure, temperature, and process medium for each application.

7. Physical Properties

7.1 *Connections*—Sight indicators are usually installed using standard pipe fittings or flanges. Pipe fittings and material should match that of the existing pipe for each installation. Type and size of fittings shall be specified in the acquisition requirements. Welding or brazing shall be performed in accordance with industry standards.

7.2 *Flanged Connections*—Where sight indicators are installed using flanges, flanges shall be in accordance with ANSI B16.5. Standard flange sizes include 1.27 cm (½ in.), 1.9 cm (¾ in.), 2.54 cm (1 in.), 3.8 cm (1-½ in.), and 5.08 cm (2 in.). Standard flange pressure ratings include 1.034 MPa (150 psi), 2.07 MPa (300 psi), and 4.14 MPa (600 psi). Other flange requirements shall be specified in the acquisition requirements.

7.3 *Vent and Drain Connections*—Where required, vent and drain connections are usually plugged, ½- or ¾-in. NPT or with NPT valves. Other vent and drain connections shall be specified in the acquisition requirements.

8. Performance Requirements

8.1 *Performance Considerations*—In many applications, certain performance characteristics are deemed critical to the intended or desired function of a sight liquid level indicator. The following are prime examples:

- (1) Accuracy,
- (2) Shock and vibration classifications, and
- (3) Operating pressure and temperature ranges.

9. Workmanship, Finish, and Appearance

9.1 *Finish and Appearance*—Any special surface finish and appearance requirements shall be specified in the acquisition requirements.

9.2 *Sight Glass Cleaning*—Any special cleaning requirements shall be specified in the acquisition requirements.

10. Inspection

10.1 *Classification of Inspections*—The inspection requirements specified herein are classified as follows:

- (1) Qualification testing and
- (2) Quality conformance testing.

10.2 *Qualification Testing*—Qualification test requirements shall be specified where applicable. Qualification test methods should be identified for each design and performance charac-

teristic specified. Test report documentation requirements should also be specified.

10.3 *Quality Conformance Testing*—Quality conformance testing is accomplished when qualification testing was satisfied by a previous acquisition or product has demonstrated reliability in similar applications. Quality conformance testing is usually less intensive than qualification, often verifying that samples of a production lot meet a few critical performance requirements.

11. Number of Tests and Retests

11.1 *Test Specimen*—The number of test specimens to be subjected to qualification testing shall depend on the design. If each range is covered by a separate and distinct design, a test specimen for each range will require testing. In instances in which a singular design series may cover multiple ranges and types, only three test specimens need be tested provided the physical similarities are approved by the buyer. In no case, however, shall less than three units, one unit each representing low, medium, and high ranges, be tested, regardless of design similarity.

12. Test Methods

12.1 *Tests*—All tests shall be performed in accordance with ASTM, ASME, or industry standards as specified.

12.2 *Test Data*—All test data shall remain on file at the manufacturer's facility for review by the buyer upon request. It is recommended that test data be retained in the manufacturer's files for at least three years or a period of time acceptable to the buyer and manufacturer.

13. Quality Assurance Provisions

13.1 *Warranty*—Unless otherwise specified, the manufacturer is responsible for the following:

- (1) All materials used to produce a unit and
- (2) Manufacturer will warrant his product to be free from defect of workmanship to produce the unit.

14. Certification

14.1 When specified in the purchase order or contract, the buyer shall be furnished certification that samples representing each lot have been either tested or inspected as directed in this specification and the requirements have been met. When specified in the purchase order or contract, a report of the test results shall be furnished.

15. Product Marking

15.1 User-specified product marking shall be listed in the acquisition requirements.

16. Packaging and Package Marking

16.1 *Packaging of Product for Delivery*—Product shall be packaged for shipment in accordance with Practice **D3951**.

16.2 Any special preservation, packaging, or package marking requirements for shipment or storage shall be identified in the acquisition requirements.

17. Keywords

17.1 direct level indicator; indirect level indicator; liquid level indicator; sight glass

SUPPLEMENTARY REQUIREMENTS

The following supplementary requirements established for U.S. Naval shipboard application shall apply when specified in the contract or purchase order. When there is conflict between the standard (Specification F2045) and this supplement, the requirements of this supplement shall take precedence for equipment acquired by this supplement. This document supersedes MIL-I-20037, Indicators, Sight, Liquid Level, Direct/Indirect Reading, Tubular Glass/Plastic, for new ship construction.

INDICATORS, SIGHT, LIQUID LEVEL, DIRECT AND INDIRECT READING, TUBULAR GLASS/PLASTIC (NAVAL SHIPBOARD USE)

S1. Scope

S1.1 This supplement covers sight liquid level indicators of the direct and indirect reading type having tubular glass, clear polycarbonate, or rigid polyvinyl chloride (PVC).

S1.2 Direct reading sight glass indicators may consist of glass or plastic tubes with fittings including shutoff valves. Indirect reading indicators may consist of a sealed chamber with a magnetic float or flag indicator.

S1.3 Indirect indicators are intended for use in water and fuel service at working pressures of 2.07 MPa (300 lb/in.²) and below, temperatures of 149°C (300°F) and below, and for hi-shock applications. Direct indicators are intended for use in hi-shock applications and shall use plastic sight tubes where the fluid is compatible and temperatures do not exceed 66°C (150°F). Glass tubes shall only be used for low shock applications and where the fluid is not compatible with plastic tubes.

S1.4 Only direct-type indicators with glass tube material less than 92 cm (36 in.) in length or indirect type indicators shall be used for hydrocarbons and flammable fluid applications.

S2. Referenced Documents

S2.1 *Commercial Documents:*

ANSI B16.5 Pipe Flanges and Flanged Fittings (DoD adopted)³

ANSI/ASQC Q9001-1994 Quality Systems—Model for Quality Assurance in Design, Development, Production, Installation, Inspection, Testing and Servicing³

ASTM A312/A312M Specification for Seamless and Welded Austenitic Stainless Steel Pipes (DoD adopted)²

ASTM B61 Specification for Steam or Valve Bronze Castings (DoD adopted)²

ASTM B62 Specification for Composition Bronze or Ounce Metal Castings (DoD adopted)²

ASTM B117 Practice for Operating Salt Spray (Fog) Apparatus²

ASTM B283 Specification for Copper and Copper-Alloy Die Forging Hot-Pressed²

ASTM D1784 Specification for Rigid Poly Vinyl Chloride PVC Compounds and Chlorinated Poly Vinyl Chloride CPVC Compounds (DoD adopted)²

ASTM D3935 Specification for Polycarbonate (PC) Unfilled and Reinforced Material²

ASTM D3951 Practice for Commercial Packaging²

MSS-SP-72 Ball Valves with Flanged or Butt-Welding Ends for General Service⁴

MSS-SP-110 Ball Valves, Threaded Socket-Welding, Solder Joint, Grooved and Flared Ends⁴

S2.2 *Government Documents:*

S2.2.1 *Military Standards:*

MIL-STD-167-1 Mechanical Vibrations of Shipboard Equipment (Type I - Environmental and Type II - Internally Excited)⁵

S2.2.2 *Military Specifications:*

MIL-S-901 Shock Tests, H.I. (High Impact); Shipboard Machinery, Equipment and Systems, Requirements for⁵

S2.2.3 *Other Government Documents:* Drawings and publications, Naval Sea Systems Command (NAVSEA)

803-5184222 Gage Glass Ball Valve⁵

S8700-1385802 Level Indicator Shield⁵

S9074-AR-GIB-010/278 Requirements for Fabrication Welding and Inspection and Casting Inspection and Repair for Machinery, Piping and Pressure Vessels⁵

S3. Terminology

S3.1 *Definitions:*

S3.1.1 *direct indication*—the tank fluid level is visible in the glass or tube.

S3.1.2 *indirect indication*—the tank fluid level is contained in a sealed chamber and indicated by some other means such as a float or flag actuated by a magnet contained in a float in the fluid chamber.

⁴ Available from Manufacturers Standardization Society of the Valve and Fittings Industry (MSS), 127 Park St., NE, Vienna, VA 22180-4602, <http://www.mss-hq.org>.

⁵ Available from DLA Document Services, Building 4/D, 700 Robbins Ave., Philadelphia, PA 19111-5094, <http://quicksearch.dla.mil>.