



Designation: D4739 – 11 (Reapproved 2017) D4739 – 17

Standard Test Method for Base Number Determination by Potentiometric Hydrochloric Acid Titration¹

This standard is issued under the fixed designation D4739; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

INTRODUCTION

Currently, there are two ASTM test methods under the jurisdiction of Committee D02 used for determining base number by potentiometric titration: Test Method D2896 and Test Method D4739. They are both used throughout the petroleum industry. Test Method D2896 is for new oils and is used in setting specifications since it is more accurate than Test Method D4739. Test Method D4739 shall be used exclusively for the purpose of tracking base number loss as an oil proceeds in service. In many cases, the test methods will provide different results. Some comparisons are given in the Scope and the Significance and Use sections of this test method to distinguish between the two standards and to provide guidance to users.

1. Scope-~~Scope~~*

1.1 This test method covers a procedure for the determination of basic constituents in petroleum products and new and used lubricants. This test method resolves these constituents into groups having weak-base and strong-base ionization properties, provided the dissociation constants of the more strongly basic compounds are at least 1000 times than that of the next weaker groups. This test method covers base numbers up to 250.

1.2 In new and used lubricants, the constituents that can be considered to have basic properties are primarily organic and inorganic bases, including amino compounds. This test method uses hydrochloric acid as the titrant, whereas Test Method D2896 uses perchloric acid as the titrant. This test method may or may not titrate these weak bases and, if so, it will titrate them to a lesser degree of completion; some additives such as inhibitors or detergents may show basic characteristics.

1.3 When testing used engine lubricants, it should be recognized that certain weak bases are the result of the service rather than having been built into the oil. This test method can be used to indicate relative changes that occur in oil during use under oxidizing or other service conditions regardless of the color or other properties of the resulting oil. The values obtained, however, are intended to be compared with the other values obtained by this test method only; base numbers obtained by this test method are not intended to be equal to values by other test methods. Although the analysis is made under closely specified conditions, this test method is not intended to, and does not, result in reported basic properties that can be used under all service conditions to predict performance of an oil; for example, no overall relationship is known between bearing corrosion or the control of corrosive wear in the engine and base number.

1.4 This test method was developed as an alternative for the former base number portion of Test Method D664 (last published in Test Method D664 – 81).

1.4.1 Colorimetric test methods for base number are Test Method D974, IP 139, and 5102.1 on acid and base number by extraction (color-indicator titration) of Federal Test Method Standard No. 791b. Test results by these methods may or may not be numerically equivalent to this test method.

1.5 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate ~~safety~~ safety, health, and ~~health~~ environmental practices and determine the applicability of regulatory limitations prior to use.*

¹ This test method is under the jurisdiction of ASTM Committee D02 on Petroleum Products, Liquid Fuels, and Lubricants and is the direct responsibility of Subcommittee D02.06 on Analysis of Liquid Fuels and Lubricants.

Current edition approved June 1, 2017/Dec. 1, 2017. Published July 2017/February 2018. Originally approved in 1987. Last previous edition approved in 2017 as D4739 – 11/D4739 – 11 (2017). DOI: 10.1520/D4739-11R17.10.1520/D4739-17.

*A Summary of Changes section appears at the end of this standard

1.7 This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.

2. Referenced Documents

2.1 ASTM Standards:²

[D664 Test Method for Acid Number of Petroleum Products by Potentiometric Titration](#)

[D974 Test Method for Acid and Base Number by Color-Indicator Titration](#)

[D1193 Specification for Reagent Water](#)

[D2896 Test Method for Base Number of Petroleum Products by Potentiometric Perchloric Acid Titration](#)

[D4057 Practice for Manual Sampling of Petroleum and Petroleum Products](#)

[D4177 Practice for Automatic Sampling of Petroleum and Petroleum Products](#)

2.2 IP Standard:³

[IP 139 Petroleum products and lubricants—Determination of acid and base number—Colour-indicator titration method](#)

2.3 U.S. Federal Test Method:⁴

[Federal Test Method Standard No. 791b Lubricants Liquid Fuels and Related Products; Methods of Testing](#)

3. Terminology

3.1 Definitions:

3.1.1 *base number, n*—the quantity of a specified acid, expressed in terms of the equivalent number of milligrams of potassium hydroxide per gram of sample, required to titrate a sample in a specified solvent to a specified endpoint using a specified detection system.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ Available from Energy Institute, 61 New Cavendish St., London, W1G 7AR, U.K., <http://www.energyinst.org>.

⁴ Available from Standardization Documents Order Desk, DODSSP, Bldg. 4, Section D, 700 Robbins Ave., Philadelphia, PA 19111-5098.

3.1.1.1 Discussion—

In this test method, the sample is titrated to a meter reading corresponding to aqueous acidic buffer solution or appropriate inflection point.

3.2 Definitions of Terms Specific to This Standard: [ASTM D4739-17](#)

3.2.1 *strong base number, n*—the quantity of acid, expressed in terms of the equivalent number of milligrams of potassium hydroxide per gram of sample, that is required to titrate a sample dissolved in the specified solvent from the initial meter reading to a meter reading corresponding to a basic buffer solution.

4. Summary of Test Method

4.1 The sample is dissolved in a mixture of toluene, propan-2-ol (isopropyl alcohol), chloroform, and a small amount of water and titrated potentiometrically with alcoholic hydrochloric acid solution. The test results of this procedure are obtained by titration mode of fixed increment and fixed time additions of the titrant. An endpoint is selected from a titration curve according to the criteria given in Section 12 and used to calculate a base number.

5. Significance and Use

5.1 New and used petroleum products can contain basic constituents that are present as additives. The relative amount of these materials can be determined by titration with acids. The base number is a measure of the amount of basic substances in the oil always under the conditions of the test. It is sometimes used as a measure of lubricant degradation in service. However, any condemning limit shall be empirically established.

5.2 As stated in 1.2, this test method uses a weaker acid to titrate the base than Test Method D2896, and the titration solvents are also different. Test Method D2896 uses a stronger acid and a more polar solvent system than Test Method D4739. As a result, Test Method D2896 will titrate salts of weak acids (soaps), basic salts of polyacidic bases, and weak alkaline salts of some metals. They do not protect the oil from acidic components due to the degradation of the oil. This test method may produce a falsely exaggerated base number. Test Method D4739 will probably not titrate these weak bases but, if so, will titrate them to a lesser degree of completion. It measures only the basic components of the additive package that neutralizes acids. On the other hand, if the additive package contains weak basic components that do not play a role in neutralizing the acidic components of the degrading oil, then the Test Method D4739 result may be falsely understated.

5.3 Particular care is required in the interpretation of the base number of new and used lubricants.

5.3.1 When the base number of the new oil is required as an expression of its manufactured quality, Test Method **D2896** is preferred, since it is known to titrate weak bases that this test method may or may not titrate reliably.

5.3.2 When the base number of in-service or at-term oil is required, this test method is preferred because in many cases, especially for internal combustion engine oils, weakly basic degradation products are possible. Test Method **D2896** will titrate these, thus giving a false value of essential basicity. This test method may or may not titrate these weak acids.

5.3.3 When the loss of base number value, as the oils proceed in service, is the consideration, this test method is to be preferred and all values including the unused oil shall be determined by this test method. Base numbers obtained by this test method shall not be related to base numbers obtained by another test method such as Test Method **D2896**.

5.3.4 In ASTM Interlaboratory Crosscheck Programs for both new and used lubricants, historically Test Method **D2896** gives a higher value for base number.

6. Apparatus

6.1 *Potentiometric Titration*, automatic or manual, with capability of adding fixed increments of titrant at fixed time intervals (see **Annex A1**).

6.1.1 The titrimer must automatically (or manually) control the rate of addition of titrant as follows: Delivery of titrant will be incremental; after delivery of precisely a 0.100 mL increment (see **6.1.2**), the delivery is stopped and a fixed time period of 90 s is allowed to pass before another 0.100 mL increment of titrant is delivered. This procedure is repeated until the titration is completed.

6.1.2 The precision of addition of the 0.100 mL increments of titrant must be ± 0.001 mL for automatic titrators. For manual buret, it should be ± 0.005 mL. A higher incremental precision is required for an automatic buret, because the total volume to the end point is summed from the individual increments; it is read from a scale with a manual buret.

6.2 *Sensing Electrode*, standard pH with glass membrane, suitable for non-aqueous titrations.

6.3 *Reference Electrode*, Silver/Silver Chloride (Ag/AgCl) reference electrode with sleeve junction, filled with 1 M to 3 M LiCl in ethanol.

6.3.1 *Combination Electrode*—Sensing electrodes may have the Ag/AgCl reference electrode built into the same electrode body, which offers the convenience of working with and maintaining only one electrode. The combination electrode shall have a sleeve junction type of reference and shall use an inert ethanol electrolyte, for example, 1 M to 3 M LiCl in ethanol. In the reference compartment, the sensing electrode part shall use a glass membrane designed for non-aqueous titrations. These combination electrodes shall have the same response or better response than a dual electrode system. They shall have removable sleeves for easy rinsing and addition of electrolyte. (**Warning**—When a movable sleeve is part of the electrode system, ensure that the sleeve is unimpaired before every titration.)

6.4 *Stirrer, Buret, Stand, Titration Vessel*, as specified in **Annex A1**, are required.

7. Reagents

7.1 *Purity of Reagents*—Reagent-grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where such specifications are available.⁵ Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

7.2 *Purity of Water*—Unless otherwise indicated, references to water shall be understood to mean reagent water that meets the requirement of either Type I, II, or III of Specification **D1193**.

7.3 *Buffer, Aqueous Acid*—Commercial pH 3 buffer solution with a tolerance of ± 0.02 pH units at 25 °C. This solution shall be replaced at regular intervals consistent with its stability or when contamination is suspected. Information related to the stability should be obtained from the manufacturer.

7.4 *Buffer, Aqueous Basic*—Commercial pH 10 buffer solution with a tolerance of ± 0.02 pH units at 25 °C. This solution shall be replaced at regular intervals consistent with its stability or when contamination is suspected. Information related to the stability should be obtained from the manufacturer.

7.5 *Chloroform*—Reagent grade. (**Warning**—Toxic and suspected carcinogen.)

7.6 *Hydrochloric Acid Solution, Standard Alcoholic (0.1 M)*—Mix 9 mL of reagent grade hydrochloric acid (HCl, sp gr 1.19) (**Warning**—Toxic and corrosive), with 1 L of anhydrous isopropyl alcohol. Standardize frequently enough to detect normality changes of 0.0005 by potentiometric titration of approximately 8 mL (accurately measured) of the 0.1 M alcoholic KOH solution diluted with 125 mL CO₂-free water.

⁵ *Reagent Chemicals, American Chemical Society Specifications*, American Chemical Society, Washington, DC. For Suggestions on the testing of reagents not listed by the American Chemical Society, see *Annual Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.

7.7 *Ethanol*—reagent grade. (**Warning**—Flammable and toxic, especially when denatured.)

7.8 *Lithium Chloride Electrolyte*—Electrolyte—Prepare a solution of 1 M to 3 M LiCl in ethanol.

7.9 *Potassium Hydroxide*—(**Warning**—Causes severe burns.)

7.10 *Potassium Hydroxide Solution, Standard Alcoholic (0.1 M)*—Add 6 g of reagent grade potassium hydroxide (KOH) (**Warning**—Toxic and corrosive), to approximately 1 L of anhydrous isopropyl alcohol. Boil gently for 10 min to effect solution. Allow the solution to stand for 2 days, and then filter the supernatant liquid through a fine sintered-glass funnel. Store the solution in a chemically resistant bottle. Dispense in a manner such that the solution is protected from atmospheric carbon dioxide (CO₂) by means of a guard tube containing soda lime or soda non-fibrous silicate absorbent, and such that it does not come into contact with cork, rubber, or saponifiable stopcock grease. Standardize frequently enough to detect normality changes of 0.0005 by potentiometric titration of weighed quantities of potassium acid phthalate dissolved in CO₂-free water.

7.11 *Propan-2-ol (Isopropyl Alcohol)*—Anhydrous, (less than 0.1 % H₂O). (**Warning**—Flammable.) If dry reagent cannot be procured, dry it by distillation through a multiple plate column, discarding the first 5 % of material distilling over and using the 95 % remaining. Also, drying can be accomplished using molecular sieves by passing the solvent upward through a molecular sieve column using one part of molecular sieve per ten parts of solvent. (**Warning**—It has been reported that, if not inhibited against it, propan-2-ol can contain peroxides. When this occurs, an explosive mixture is possible when the storage vessel or other equipment such as a dispensing bottle, are near empty and approaching dryness.

7.12 Commercially available solutions may be used in place of laboratory preparations provided the solutions have been certified as equivalent.

7.13 Alternate volumes of solutions may be prepared provided the final solution concentration is equivalent.

7.14 *Toluene*—Reagent grade. (**Warning**—Extremely flammable.)

7.15 *Titration Solvent*—In a brown reagent bottle, add 30 mL of water to 1 L of isopropyl alcohol, and mix thoroughly. Add 1 L each of toluene and chloroform, and mix thoroughly.

8. Preparation of Electrode System

8.1 *Maintenance and Storage of Electrodes*—Cleaning the electrode thoroughly, keeping the ground-glass joint free of foreign materials, and regular testing of the electrodes are very important in obtaining repeatable potentials, since the contamination may introduce uncertain erratic and unnoticeable liquid contact potentials. While this is of secondary importance when end points are chosen from inflection points in the titration curve, it may be very serious when end points are chosen at experimentally determined cell potentials as outlined in the procedure.

8.1.1 Clean the pH indicating electrode or the pH indicating part of the combination electrode at frequent intervals based on use and type of samples being analyzed by immersing in non-chromium containing, strongly oxidizing cleaning solution. The electrode shall be cleaned periodically when in use or when a new electrode is installed. Drain the LiCl electrolyte from the electrode at least once each week, and refill with fresh LiCl electrolyte as far as the filling hole. Ensure that there are no air bubbles in the electrode liquid. If air bubbles are observed, hold the electrode in a vertical position and gently tap it to release the bubbles. Maintain the electrolyte level in the electrode above that of the liquid in the titration beaker at all times.

8.1.2 When not in use, immerse the lower halves of the electrodes in either water (sensing) or the LiCl in isopropyl alcohol electrolyte (reference). Do not allow them to remain immersed in titration solvent for any appreciable period of time between titrations. While the electrodes are not extremely fragile, handle them carefully at all times.

8.1.3 *Electrode Life*—Typically, electrode usage is limited to 3 to 6 months, depending upon usage. Electrodes have a limited shelf life and shall be tested before use (8.3).

8.2 Preparation of Electrodes:

8.2.1 When Ag/AgCl reference electrode is used for the titration and it contains an electrolyte that is not 1 M to 3 M LiCl in ethanol, replace the electrolyte. Drain the electrolyte from the electrode, wash away all the salt (if present) with water and then rinse with ethanol. Rinse several times with the LiCl electrolyte solution. Finally, replace the sleeve and fill the electrode with the LiCl electrolyte to the filling hole. When refitting the sleeve, ensure that there will be a free flow of electrolyte into the system. A combination electrode shall be prepared in the same manner. The electrolyte in a combination electrode can be removed with the aid of a vacuum suction.

8.2.2 Prior to each titration, soak the prepared electrodes in water, pH 4.5 – 5.5 acidified with HCL, for at least ~~5 min.~~ 5 min. Rinse the electrode with propan-2-ol immediately before use, and then with the titration solvent.

8.3 *Testing of Electrodes*—See [Appendix X2](#) for the procedure to check electrode performance.

9. Standardization of Apparatus

9.1 *Determination of Meter Readings for the Aqueous Buffer Solution*—Ensure comparable selection of end points when definite inflection points are not obtained in the titration curve. Determine daily, for each electrode pair, the meter readings obtained with

the aqueous acidic buffer solution to be used for the determination of base numbers and with the aqueous basic buffer solution to be used for the determination of strong base numbers.

9.2 Prepare the electrodes as described in 8.2, immerse them in the appropriate aqueous buffer solution, and stir for at least 2 min, maintaining the temperature of the buffer solution at a temperature within 2 °C of that at which the titrations are to be made. Read the cell voltage. The reading so obtained in the acidic buffer solution is taken as the end point for the base number if an inflection is not observed as specified in 12.1, and the reading obtained in the basic buffer solution is taken as the end point for the strong base number.

10. Preparation of Sample of Used Oil

10.1 ~~Strict observation of the sampling procedure~~When applicable, refer to Practice [D4057](#) is necessary, since the sediment itself is acidic or basic or (Manual Sampling) or Practice [D4177](#) has absorbed acidic or basic material from the sample. Failure to obtain a representative sample causes serious errors. (Automatic Sampling) for proper sampling techniques.

10.1.1 ~~When applicable, refer to Practices~~sampling used lubricants, the [D4057](#) (Manual Sampling) or Practicespecimen shall be representative of [D4177](#) (Automatic Sampling) for proper sampling techniques:the system sampled and shall be free of contamination from external sources.

10.1.2 ~~When sampling used lubricants, the specimen shall be representative of the system samples and shall be free of contamination from external sources. As used oil can change appreciably in storage, test samples as soon as possible after removal from the lubricating system, and note the dates of sampling and testing.~~Agitate used oil samples thoroughly to ensure that any sediment present is homogeneously suspended before analysis, as the sediment can be acidic or basic or have adsorbed acidic or basic material from the sample. When necessary, samples are warmed to aid mixing.

NOTE 1—As used oils can change appreciably in storage, samples should be tested as soon as possible after removal from the lubricating system and the dates of sampling and testing, if known, should be noted.

10.2 ~~Heat the sample (Note 1) of used oil to 60 °C ± 5 °C in the original container, and agitate the sample until all of the sediment is homogeneously suspended in the oil. If the original container is a can, or if it is glass and more than three-fourths full, transfer the entire sample to a clear glass bottle having a capacity at least one-third greater than the volume of the sample. Transfer all traces of sediment from the original container to the bottle by vigorous agitation of portions of the sample in the original container.~~

10.3 ~~After complete suspension of all sediment, strain the sample or a convenient aliquot through a 100 mesh screen for the removal of large particles.~~

NOTE 1—When samples are visibly free of sediment, the heating procedures described may be omitted.

11. Procedure for Base Number and Strong Base Number [D4739-17](#)

11.1 Calculate the quantity of sample required for its expected base number as follows:

$$A = 7/E \quad (1)$$

where:

A = approximate mass of sample, g and

E = expected base number.

11.1.1 Take a maximum of 5 g and a minimum of 0.1 g for analysis. The precision of weighing is as follows:

Size of Sample, g	Precision of Weighing, g
1–5	0.005
0.1–1	0.002


11.2 Into a suitable titration vessel, introduce a weighed quantity of sample as prescribed in 11.1.1, and add 75 mL of titration solvent. If 75 mL of solvent is not sufficient to properly cover the electrodes, add just enough additional solvent to do so. Ensure the electrodes are properly immersed. Prepare the electrodes as directed in 8.2. Place the beaker or titration vessel on the titration stand, and adjust its position so that the electrodes are about half immersed. Start the stirrer, and stir throughout the determination at a rate sufficient to produce vigorous agitation without spattering and without stirring air into the solution.

11.3 Select and fill a suitable buret with the 0.1 M alcoholic HCl solution, and place the buret in position on the titration assembly, taking care that the tip is immersed about 25 mm in the liquid in titration vessel. Record the initial buret and meter (cell potential) readings.

11.4 *Titration*—The reaction of the hydrochloric acid with the basic components is very slow with most titrations for base number. As a result, these titrations are not at equilibrium. Because of this, the titration conditions are tightly specified and must be strictly adhered to in order to achieve the precision as stated.

NOTE 2—When best precision of titration is desired, if the titrant tip has been sitting for more than 30 min without being used, it is best to purge the tips by dispensing a few millilitres of titrant before beginning a titration.

NOTE 3—See [Appendix X1](#) for techniques for reducing the titration time of a sample. Pre-dosing techniques have been found to provide satisfactory

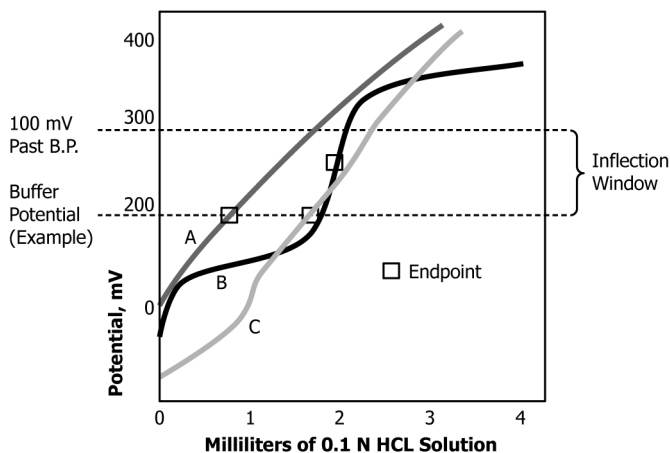

- (A) Titration curve has no inflections. Take end point at the buffer potential.
- (B) Titration curve has well-defined inflection within prescribed window. Take well-defined inflection as the end point.
- (C) Titration curve has inflection prior to buffer potential but not in prescribed window. Take end point at buffer potential.

FIG. 1 Example Titration Curves to Illustrate Selection of End Points

results, although the precision using these techniques has not been determined.

11.4.1 Whether the titration is carried out manually or automatically, the following procedure of *fixed increment, fixed time* addition of titrant shall be followed. Add 0.1 M HCl in increments of 0.100 mL throughout the titration with a 90 s pause between each incremental addition. Take millivolt readings at the end of each 90 s interval.

11.4.1.1 The meter readings of potential difference are plotted manually or automatically against the respective volumes of titrant, and the end point is taken as described in 12.1.

11.4.2 On completion of the titration, remove the titration vessel and rinse the electrodes and buret tip with the titration solvent, then with water, then again with titration solvent. (*Soak electrodes in distilled water for at least 5 min before using for another titration.*) Store the sensing electrode in deionized or distilled water and the reference electrode in a saturated solution of LiCl in isopropyl alcohol when not in use (see 8.1).

11.4.3 *Blanks*—For each set of samples, make a blank titration of the same volume of titration solvent used for the sample. For the base number blank, add 0.1 M alcoholic HCl solution in 0.01 mL increments, waiting 12 s between each addition, until a potential which is 100 mV past the buffer potential (see 11.4) is reached. For the strong base number blank, add KOH titrant under the same conditions until the potential corresponding to the basic buffer solution is reached.

12. Calculation

12.1 If an inflection (see Note 4) occurs in the potential region between the pH 3 buffer potential (see 11.4) and a point 100 mV past this potential, mark this inflection as the end point. If more than one inflection points are observed, use the last well-defined inflection point. If no well-defined inflection occurs in the above mentioned potential region, mark as the end point the point on the curve that corresponds to the acidic aqueous pH 3 buffer potential. See Fig. 1 for examples of end points.

NOTE 4—An inflection point is generally recognizable by inspection whenever at least five successive cell potential changes, Δ , caused by the addition of the corresponding five increments of titrant, exhibit a maximum illustrated as follows:

Titrant, mL	Δ , mV
1.8	8.3
1.9	10.7
2.0	11.3
2.1	10.0
2.2	7.9

The Δ at the maximum should be at least 5 mV, and the difference in Δ between the maximum and both the first and last Δ should be at least 2 mV.

12.2 Calculate the base number and strong base number as follows:

$$\text{Base number, mg KOH/g} = [(A - B) \times M \times 56.1] / W \tag{2}$$

$$\text{Strong base number, mg KOH/g} = [(CM + Dm) \times 56.1] / W \tag{3}$$

where:

- A = alcoholic HCl solution, mL, used to titrate the sample to the end point (aqueous acidic pH 3 buffer or inflection—see 7.3 and 12.1),
- B = alcoholic HCl, mL, used to titrate the solvent blank to the same potential at which the sample end point occurs,