



Designation: **E2736 – 10** **E2736 – 17**

Standard Guide for Digital Detector Array RadiologyRadiography¹

This standard is issued under the fixed designation E2736; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ε) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This standard is a user guide, which is intended to serve as a tutorial for selection and use of various digital detector array systems nominally composed of the detector array and an imaging system to perform digital radiography. This guide also serves as an in-detail reference for the following standards: Practices **E2597**, **E2698**, and **E2737**.

1.2 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate ~~safety~~ safety, health, and ~~health~~ environmental practices and determine the applicability of regulatory limitations prior to use.*

1.3 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 ASTM Standards:²

E94 Guide for Radiographic Examination Using Industrial Radiographic Film

E155 Reference Radiographs for Inspection of Aluminum and Magnesium Castings

E192 Reference Radiographs of Investment Steel Castings for Aerospace Applications

E747 Practice for Design, Manufacture and Material Grouping Classification of Wire Image Quality Indicators (IQI) Used for Radiology

E1000 Guide for Radioscopy

E1025 Practice for Design, Manufacture, and Material Grouping Classification of Hole-Type Image Quality Indicators (IQI) Used for Radiology

E1316 Terminology for Nondestructive Examinations

E1320 Reference Radiographs for Titanium Castings

E1742 Practice for Radiographic Examination

E1815 Test Method for Classification of Film Systems for Industrial Radiography

E1817 Practice for Controlling Quality of Radiological Examination by Using Representative Quality Indicators (RQIs)

E2002 Practice for Determining Total Image Unsharpness and Basic Spatial Resolution in Radiography and Radioscopy

E2422 Digital Reference Images for Inspection of Aluminum Castings

E2445 Practice for Performance Evaluation and Long-Term Stability of Computed Radiography Systems

E2446 Practice for Manufacturing Characterization of Computed Radiography Systems

E2597 Practice for Manufacturing Characterization of Digital Detector Arrays

E2660 Digital Reference Images for Investment Steel Castings for Aerospace Applications

E2669 Digital Reference Images for Titanium Castings

E2698 Practice for Radiological Examination Using Digital Detector Arrays

E2737 Practice for Digital Detector Array Performance Evaluation and Long-Term Stability

2.2 ISO Document:³

ISO 17636-2 Non-Destructive Testing of Welds—Radiographic Testing - Part 2: X- and Gamma-Ray Techniques with Digital Detector

¹ This guide is under the jurisdiction of ASTM Committee **E07** on Nondestructive Testing and is the direct responsibility of Subcommittee **E07.01** on Radiology (X and Gamma) Method.

Current edition approved April 15, 2010Dec. 1, 2017. Published July 2010February 2018. Originally approved in 2010. Last previous edition approved in 2010 as E2736 – 10. DOI: 10.1520/E2736-17.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For Annual Book of ASTM Standards volume information, refer to the standard's Document Summary page on the ASTM website.

³ Available from International Organization for Standardization (ISO), ISO Central Secretariat, BIBC II, Chemin de Blandonnet 8, CP 401, 1214 Vernier, Geneva, Switzerland, <http://www.iso.org>.

3. Terminology

3.1 Definitions of Terms Specific to This Standard:

3.1.1 *digital detector array (DDA) system*—an electronic device that converts ionizing or penetrating radiation into a discrete array of analog signals which are subsequently digitized and transferred to a computer for display as a digital image corresponding to the radiation energy pattern imparted upon the input region of the device. The conversion of the ionizing or penetrating radiation into an electronic signal may transpire by first converting the ionizing or penetrating radiation into visible light through the use of a scintillating material. These devices can range in speed from many minutes per image to many images per second, up to and in excess of real-time radioscopes rates (usually 30 frames per seconds).

3.1.2 *signal-to-noise ratio (SNR)*—quotient of mean value of the intensity (signal) and standard deviation of the intensity (noise). The SNR depends on the radiation dose and the DDA system properties.

3.1.3 *normalized signal-to-noise ratio (SNR_N)*—SNR normalized for basic spatial resolution (see Practice E2445).

3.1.4 *basic spatial resolution (SR_b)*—basic spatial resolution indicates the smallest geometrical detail, which can be resolved using the DDA. It is similar to the effective pixel size.

3.1.5 *efficiency*—dSNR_N (see 3.1.6 of Practice E2597) divided by the square root of the dose (in mGy) and is used to measure the response of the detector at different beam energies and qualities.

3.1.1 *achievable contrast sensitivity (CS_a)*—~~optimum~~^{best} contrast sensitivity (see Terminology E1316 for a definition of contrast sensitivity) obtainable using a standard phantom with an X-ray technique that has little contribution from scatter.

3.1.7 *specific material thickness range (SMTR)*—material thickness range within which a given image quality is achieved.

3.1.2 *contrast-to-noise ratio (CNR)*—~~bad pixel~~—quotient of the difference of the mean signal levels between two image areas and the standard deviation of the signal levels. The CNR depends on the radiation dose and the DDA system properties. a bad pixel is a pixel identified with a performance outside of the specification for a pixel of a DDA as defined in Practice E2597.

3.1.9 *lag*—residual signal in the DDA that occurs shortly after the exposure is completed.

3.1.3 *burn-in*—change in gain of the scintillator or photoconductor that persists well beyond the exposure.

3.1.11 *internal scatter radiation (ISR)*—scattered radiation within the detector (from scintillator, photodiodes, electronics, shielding, or other detector hardware).

3.1.4 *bad pixel—efficiency*—a ~~SNR_N~~ bad pixel is a pixel identified with a performance outside of the (see 3.1.6 of Practice E2597) specification for a pixel of a DDA as defined in Practice E2597. ~~and is used to measure the response of the detector at different beam energies and qualities.~~

3.1.5 *grooved wedge*—a wedge with one groove, that is 5 % of the base material thickness and that is used for achievable contrast sensitivity measurement in Practice E2597. ASTM E2736-17

3.1.6 *internal scatter radiation (ISR)*—scattered radiation within the detector (from scintillator, photodiodes, electronics, shielding, or other detector hardware).

3.1.7 *lag*—residual signal in the DDA that occurs shortly after the exposure is completed.

3.1.8 *phantom*—a part or item being used to quantify DDA characterization metrics.

3.1.9 *SNR_N*—SNR, normalized by the basic spatial resolution SR_b as measured directly in the digital image and/or calculated from measured SNR_{measured} by:

$$SNR_N = SNR_{measured} \times \left(\frac{88.6 \mu m}{SR_b} \right) \quad (1)$$

3.1.10 *specific material thickness range (SMTR)*—material thickness range within which a given image quality is achieved.

4. Significance and Use

4.1 This standard provides a guide for the other DDA standards (see Practices E2597, E2698, and E2737). It is not intended for use with computed radiography apparatus. Figure 1 describes how this standard is interrelated with the aforementioned standards.

4.2 This guide is intended to assist the user to understand the definitions and corresponding performance parameters used in related standards as stated in 4.1 in order to make an informed decision on how a given DDA can be used in the target application.

4.3 This guide is also intended to assist cognizant engineering officers, prime manufacturers, and the general service and manufacturing customer base that may rely on DDAs to provide advanced radiological results so that these parties may set their own acceptance criteria for use of these DDAs by suppliers and shops to verify that their parts and structures are of sound integrity to enter into service.

4.4 The manufacturer characterization standard for DDA (see Practice E2597) serves as a starting point for the end user to select a DDA for the specific application at hand. DDA manufacturers and system integrators will provide DDA performance data using

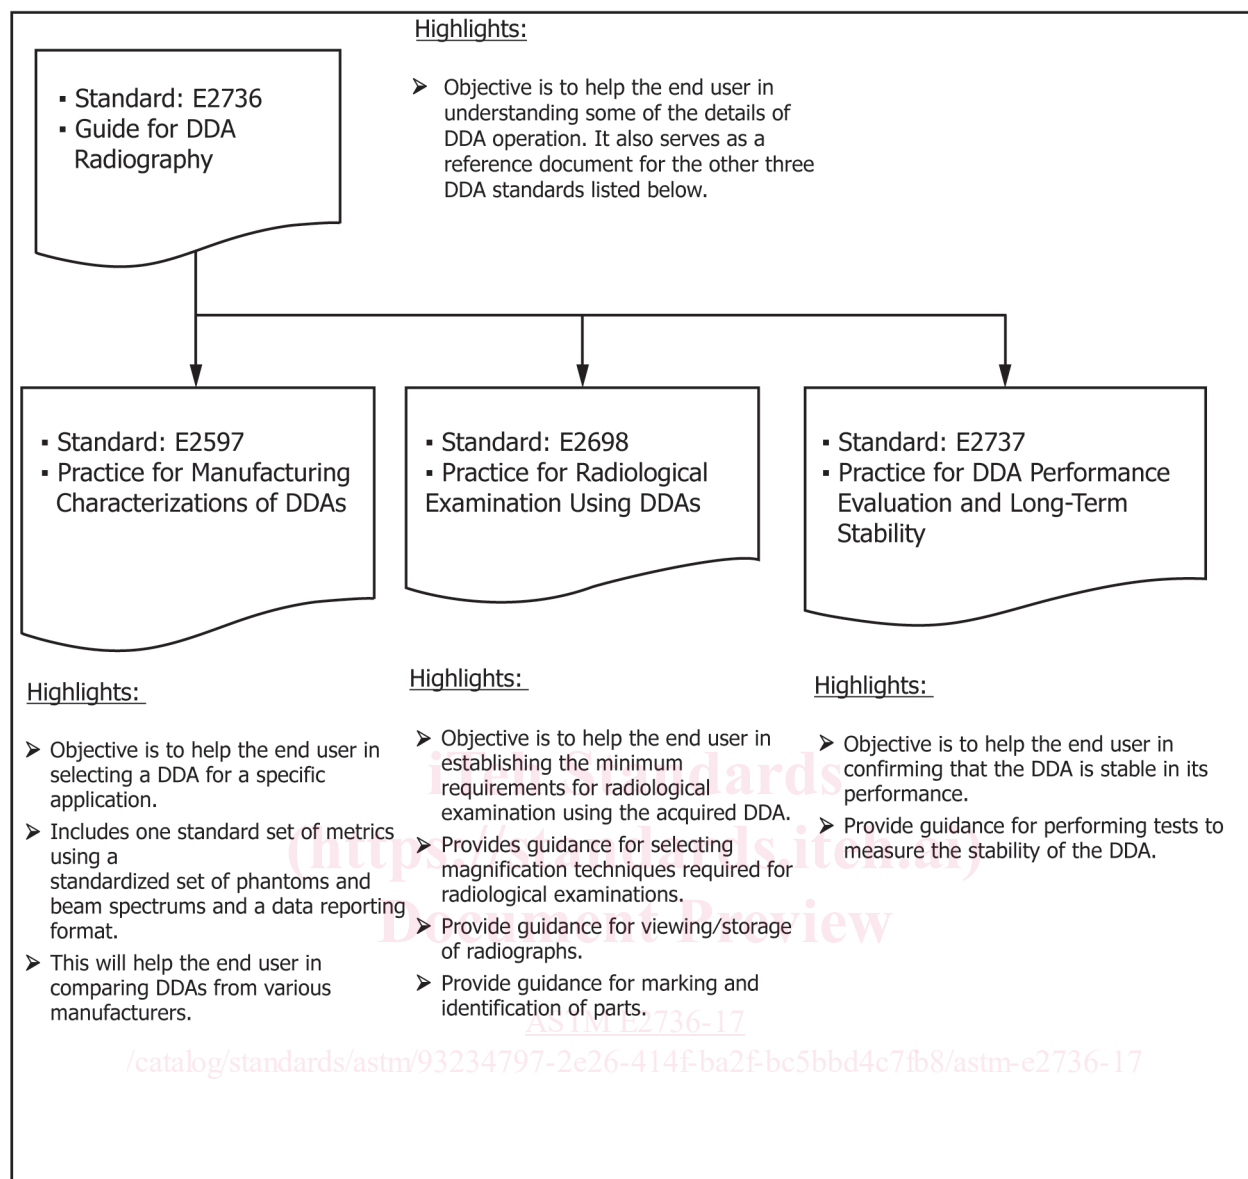


FIG. 1 Flow Diagram Representing the Connection Between the Four DDA Standards

standardized geometry, X-ray beam spectra, and phantoms as prescribed in Practice **E2597**. The end user will look at these performance results and compare DDA metrics from various manufacturers and will decide on a DDA that can meet the specification required for inspection by the end user. See Sections 5 and 8 for a discussion on the characterization tests and guidelines for selection of DDAs for specific applications.

4.5 Practice **E2698** is designed to assist the end user to set up the DDA with minimum requirements for radiological examinations. This standard will also help the user to get the required SNR, to set up the required magnification, and provides guidance for viewing and storage of radiographs. Discussion is also added to help the user with marking and identification of parts during radiological examinations.

4.6 Practice **E2737** is designed to help the end user with a set of tests so that the stability of the performance of the DDA can be confirmed. Additional guidance is provided in this document to support this standard.

4.7 Figure 1 provides a summary of the interconnectivity of these four DDA standards.

4.8 DDAs may be used with significant success under a wide energy range, i.e. from 10 kV to 20 MeV if configured appropriately. However in this document some phantoms such as the duplex wire gauge (Practice **E2002**) may not give an accurate representation of the basic spatial resolution at energies above 600 kV.