
Anaesthetic vaporizers — Agent-specific filling systems

Évaporateurs d'anesthésie — Systèmes de remplissage spécifiques à l'agent

Sample Document

get full document from standards.iteh.ai



Reference number
ISO 5360:2016(E)

© ISO 2016

Sample Document

get full document from standards.iteh.ai



COPYRIGHT PROTECTED DOCUMENT

© ISO 2016, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Bottle	2
5 Bottle collar	3
6 Bottle adaptor	6
7 Filler receptacle	10
8 Filling rate	12
9 Leakage	14
10 Overfilling protection	14
11 Colour coding	14
12 Usability	14
13 Clinical evaluation	14
14 Information provided by the manufacturer	15
14.1 Marking.....	15
14.2 Labelling.....	15
14.3 Instructions for use.....	15
Annex A (informative) Recommendations on materials	17
Annex B (informative) Types of agent-specific filling systems	18
Annex C (normative) Determination of total leakage into atmosphere of anaesthetic agent during filling	19
Bibliography	21

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#).

The committee responsible for this document is ISO/TC 121, *Anaesthetic and respiratory equipment*, Subcommittee SC 1, *Breathing attachments and anaesthetic machines*.

This fourth edition cancels and replaces the third edition (ISO 5360:2012), of which it constitutes a minor revision with the following changes:

- [Figure 5](#) has been technically revised;
- minor editorial modifications have been incorporated into the text.

Anaesthetic vaporizers — Agent-specific filling systems

1 Scope

This International Standard specifies requirements, including dimensions, for agent-specific filling systems for agent-specific anaesthetic vaporizers.

This International Standard does not specify construction materials.

NOTE 1 For recommendations on materials, see [Annex A](#).

Because of the unique properties of desflurane, dimensions for this agent have not been specified in this International Standard.

NOTE 2 Designs of connection systems, which only permit engagement of the agent-specific bottle adaptor to the bottle when the bottle collar is in place, are encouraged.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1101, *Geometrical Product Specifications (GPS) — Geometrical tolerancing — Tolerances of form, orientation, location and run-out*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

agent-specific

having both a prescribed configuration and prescribed dimensions, which are specific for a prescribed liquid anaesthetic agent

3.2

agent-specific filling system

functional system of *agent-specific* (3.1) coded connections between an anaesthetic bottle and an *agent-specific* (3.1) anaesthetic vaporizer (3.3), consisting of, for example, a threaded *bottle neck* (3.7) with collar, *bottle connector* (3.6), *male adaptor* (3.9), and *filler receptacle* (3.8)

Note 1 to entry: Different types of agent-specific filling systems are shown in [Annex B](#).

3.3

anaesthetic vaporizer

device designed to facilitate the change of an anaesthetic agent from a liquid to a vapour

3.4

bottle adaptor

assembly that is intended to connect a bottle for liquid anaesthetic agent to an *agent-specific* (3.1) anaesthetic vaporizer (3.3)

3.5

bottle collar

agent-specific (3.1) component on the neck of a bottle causing it to be *agent-specific* (3.1)

3.6

bottle connector

agent-specific (3.1) component that fits the thread on the *bottle neck* (3.7) and mates with the *agent-specific* (3.1) *bottle collar* (3.5)

3.7

bottle neck

external threaded part of the bottle and the adjacent contour over which an *agent-specific* (3.1) collar is fitted

3.8

filler receptacle

receptacle for a bottle or a *bottle adaptor* (3.4) on an *agent-specific* (3.1) *anaesthetic vaporizer* (3.3)

3.9

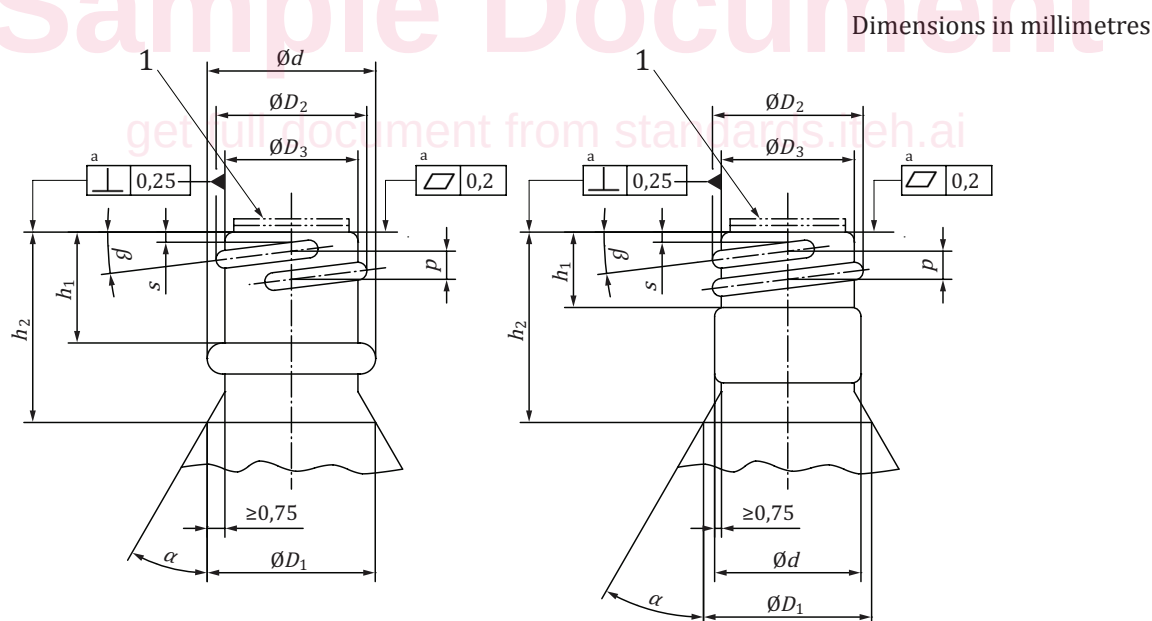
male adaptor

part of a *bottle adaptor* (3.4) that mates with a *filler receptacle* (3.8) on an *agent-specific* (3.1) vaporizer

4 Bottle

Each bottle shall have the following:

- name of the anaesthetic agent with which it is intended to be used marked on it;
- either a bottle collar complying with [Clause 5](#) and a threaded neck complying with [Figure 1](#) and [Table 1](#), or a permanently attached bottle adaptor complying with [6.2](#).

**Key**

- 1 optional pouring lip (dimension not specified)
- a Flatness and perpendicularity tolerances in accordance with ISO 1101.

NOTE The dimensions shown form part of this International Standard. Other features are for illustrative purposes only. See [Table 1](#).

Figure 1 — Two examples of threaded necks of bottles for anaesthetic agents

Table 1 — Dimensions of threaded necks of bottles for anaesthetic agents

Bottle type	Anaesthetic agent	h_1 ±0,3 mm	h_2^a min. mm	s ±0,45 mm	β	α min. at $\varnothing D_1$	p mm	Thread turns min.	D_1^a nom. mm	D_2^b ±0,3 mm	D_3^b ±0,3 mm	d max. mm
1	Isoflurane Enflurane	9,75	23	1,2	2° 35'	30°	3,2	1	28	23,6	21,5	28
2	Halothane	6,8	18,7	1,2	2° 15'	30°	2,54	1,25	24	21,45	19,7	28
3	Halothane (USA)	15	26,3	1	2° 50'	30°	3,2	1,75	24	21,7	19,5	28
4	Spare	9,05	20	1,15	3° 30'	30°	3,2	1,25	20	17,65	15,5	28
5	Spare	9,05	20	1,15	3° 7'	30°	3,2	1,25	22	19,65	17,5	28
6	Methoxy- flurane	9,8	20	1,15	2° 57'	30°	4,25	1,25	30	27,3	24,9	32
7	Spare	9,85	20	1,15	2° 31'	30°	4,25	1,25	34	31,8	29,4	32
8	Sevoflurane	8,9	23,9	1,3	2° 56'	30°	3,63	1,25	23,9	23,5	21,5	28

NOTE See [Figure 1](#).^a Recommended values.^b Summation of the tolerances of measures D_2 and D_3 shall be avoided. A maximum tolerance of ±0,3 mm for $(D_2 - D_3)$ should be required to avoid problems with the fitting of any bottle connector.

5 Bottle collar

5.1 Bottle collars shall comply with the configuration and dimensions shown in [Figure 2](#) and angle, θ , specified in [Table 2](#) for the anaesthetic agent with which it is intended to be used.

5.2 The position of the bottle collar relative to the screw thread of the bottle shall be as shown in [Figure 3](#).

5.3 The bottle collar shall be attached to the bottle and shall be rotatable by hand.