
**Human response to vibration —
Measuring instrumentation —**

**Part 1:
General purpose vibration meters**

*Réponse des individus aux vibrations — Appareillage de mesure —
Partie 1: Instrument de mesure à usage général*

Sample Document

get full document from standards.iteh.ai



Sample Document

get full document from standards.iteh.ai



COPYRIGHT PROTECTED DOCUMENT

© ISO 2017, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	vi
Introduction	vii
1 Scope	1
2 Normative references	1
3 Terms, definitions and symbols	2
3.1 Terms and definitions	2
3.1.1 General	2
3.1.2 Frequency-weighted values	4
3.2 Symbols	6
4 Reference environmental conditions	8
5 Performance specifications	8
5.1 General characteristics	8
5.2 Display of signal magnitude	10
5.2.1 General	10
5.2.2 Resolution and refresh rate	10
5.2.3 Stabilization, measurement start and display times	11
5.3 Electrical output	11
5.4 Vibration sensitivity	11
5.5 Accuracy of indication at reference frequency under reference conditions	12
5.6 Frequency weightings and frequency responses	12
5.6.1 Parameters	12
5.6.2 Band-limiting filter	13
5.6.3 a-v transition filter	13
5.6.4 Upward-step filter	14
5.6.5 Overall frequency weighting	14
5.6.6 Tolerances	14
5.7 Amplitude linearity	15
5.8 Instrument noise	16
5.9 Signal-burst response	16
5.10 Overload indication	19
5.11 Under-range indication	20
5.12 Time averaging	20
5.13 Running r.m.s. acceleration	20
5.14 Reset	21
5.15 Timing facilities	21
5.16 Electrical cross-talk	21
5.17 Vibration transducer characteristics	21
5.18 Power supply	21
6 Mounting	22
7 Environmental and electromagnetic criteria	22
7.1 General	22
7.2 Air temperature	22
7.3 Surface temperature	23
7.4 Electrostatic discharge	23
7.5 Radio-frequency emissions and public-power-supply disturbances	23
7.6 Immunity to AC power-frequency fields and radio-frequency fields	24
7.7 Ingress of water and dust	24
8 Provision for use with auxiliary devices	25
9 Instrument marking	25
10 Instrument documentation	25

11	Testing and calibration	25
12	Pattern evaluation	28
12.1	General	28
12.2	Testing requirements	28
12.3	Submission for testing	29
12.4	Marking of the vibration meter and information in the instrument documentation	29
12.5	Mandatory facilities and general requirements	29
12.6	Initial instrument preparation	29
12.7	Indication at the reference frequency under reference conditions	29
12.8	Electrical cross-talk	30
12.9	Vibration transducer	30
12.10	Amplitude linearity and under-range indication	31
12.10.1	Electrical tests of amplitude linearity	31
12.10.2	Mechanical tests of amplitude linearity	32
12.11	Frequency weightings and frequency responses	33
12.11.1	General	33
12.11.2	Mechanical tests of frequency response	33
12.11.3	Electrical tests of frequency response	34
12.11.4	Conformance	35
12.12	Instrument noise	35
12.13	Signal-burst response	36
12.14	Overload indication	36
12.15	Reset	36
12.16	Combined axis outputs	37
12.17	AC electrical output	37
12.18	Timing facilities	37
12.19	Power supply	37
12.20	Environmental, electrostatic and radio-frequency tests	37
12.20.1	General	37
12.20.2	Expanded uncertainties for measurements of environmental conditions	38
12.20.3	Acclimatization requirements for tests of the influence of air temperature and relative humidity	38
12.20.4	Test of the influence of air temperature and relative humidity combined	38
12.20.5	Influence of surface temperature	39
12.20.6	Influence of electrostatic discharges	39
12.20.7	Radio-frequency emissions and public-power-supply disturbances	39
12.20.8	Immunity to AC power-frequency fields and radio-frequency fields	40
12.21	Test report	41
13	Validation of one-off instruments	42
13.1	General	42
13.2	Testing requirements	42
13.3	Test object	42
13.4	Submission for testing	43
13.5	Marking of the one-off instrument and information in the instrument documentation	43
13.6	Mandatory facilities and general requirements	43
13.7	Initial instrument preparation	43
13.8	Test procedure	43
13.9	Indication at the reference frequency under reference conditions	44
13.10	Test parameters	45
13.10.1	Vibration measurement chain for hand-arm vibration	45
13.10.2	Vibration measurement chain for whole-body vibration	45
13.10.3	Vibration measurement chain low-frequency whole-body vibration	46
13.11	Conducting the test	46
13.12	Instrument noise	47
13.13	Electrical cross-talk	47
13.14	Overload indication	47
13.15	Timing facilities	47

13.16	Test report.....	48
14	Periodic verification	48
14.1	General.....	48
14.2	Testing requirements	48
14.3	Test object.....	48
14.4	Submission for testing.....	48
14.5	Preliminary inspection.....	49
14.6	Marking of the vibration meter and information in the instrument documentation	49
14.7	Test procedure.....	49
14.8	Test parameters.....	50
14.8.1	Vibration measurement chain for hand-arm vibration.....	50
14.8.2	Vibration measurement chain for whole-body vibration.....	50
14.8.3	Vibration measurement chain low-frequency whole-body vibration.....	50
14.9	Conducting the test	51
14.10	Test report.....	51
15	<i>In situ</i> checks	51
15.1	General.....	51
15.2	Preliminary inspection.....	52
15.3	Vibration sensitivity (field calibration).....	52
	Annex A (normative) Specification for field vibration calibrator	53
	Annex B (informative) Frequency weightings.....	55
	Annex C (informative) Realization of frequency weighting filters	74
	Annex D (informative) Running r.m.s. time averaging.....	78
	Annex E (informative) Vibration transducer characteristics.....	81
	Annex F (informative) Tests for mounting systems	84
	Annex G (normative) Instrument documentation.....	87
	Annex H (normative) Phase response requirements for measurement of non-r.m.s. quantities.....	92
	Annex I (informative) Guidelines for the estimation of the instrumental measurement uncertainty.....	100
	Bibliography	106

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 108, *Mechanical vibration, shock and condition monitoring*, Subcommittee SC 3, *Use and calibration of vibration and shock measuring instruments*.

This first edition cancels and replaces ISO 8041:2005, which has been technically revised. It also incorporates the Technical Corrigendum ISO 8041:2005/Cor. 1:2007. The following main changes have been made:

- addition of an Introduction explaining the reasons for this revision;
- addition of a validation test for one-off instruments;
- revision and simplification of the verification test;
- addition of Annex I, which gives example estimates of the instrumental measurement uncertainty;
- correction of errors in formulae, numbers and figures.

A list of parts in the ISO 8041 series can be found on the ISO website.

Introduction

Until 2005, when the previous edition of this document was published, measuring instrumentation for human response to vibration (vibration meters) normally consisted of a signal processing unit and a detachable vibration transducer. According to recent developments, however, part of the signal processing steps can be integrated in the transducer unit, so that the signal coming out of the transducer's sensing element and going into the signal conditioning unit is not accessible any more. These transducer units include, for example, IEPE and MEMS transducers.

Some of the test procedures specified in this document, however, presume that this point in the signal path is accessible (electrical input). Since such an input is not mandatory these tests can only be performed on a vibration meter having an electrical input or after some technical modifications to the instrumentation, e.g. internal access to signal paths. Or those tests can only be performed mechanically, which in certain cases requires modifications to some test procedures. Such modifications to test procedures, however, are beyond the present scope of this document.

Some of the test procedures specified in this document can only be performed if an electrical output is available, see for example [5.13](#). Since such an output is not mandatory these tests can only be performed on a vibration meter having an electrical output or after some technical modifications to the instrumentation, e.g. internal access to signal paths.

The verification test now specified in this document is practicable and has the objective of identifying an instrument which is adequately calibrated for the intended applications and is suitable for its purpose, at a cost reasonable for the calibration laboratory and affordable for the end user. Therefore, the verification test is strongly reduced in its extent compared to the full pattern evaluation, or validation, and only tests the most relevant characteristics of a vibration meter.

Sample Document

get full document from standards.iteh.ai

Sample Document

get full document from standards.iteh.ai

Human response to vibration — Measuring instrumentation —

Part 1: General purpose vibration meters

1 Scope

This document specifies the performance specifications and tolerance limits for instruments designed to measure vibration values, for the purpose of assessing human response to vibration. It includes requirements for pattern evaluation, or validation, periodic verification and *in situ* checks, and the specification of vibration calibrators for *in situ* checks.

Vibration instruments specified in this document can be single instruments, combinations of instrumentation or computer-based acquisition and analysis systems.

Vibration instruments specified in this document are intended to measure vibration for one or more applications, such as the following:

- hand-transmitted vibration (see ISO 5349-1);
- whole-body vibration (see ISO 2631-1, ISO 2631-2 and ISO 2631-4);
- low-frequency whole-body vibration in the frequency range from 0,1 Hz to 0,5 Hz (see ISO 2631-1).

Vibration instruments can be designed for measurement according to one or more of the frequency weightings defined within each of these applications.

Three levels of performance testing are defined in this document:

- a) pattern evaluation or validation:
 - 1) pattern evaluation, i.e. a full test of the instrument against the specifications defined in this document;
 - 2) validation of one-off instruments, i.e. a limited set of tests of an individual vibration measuring system against the relevant specifications defined in this document;
- b) periodic verification, i.e. an intermediate set of tests designed to ensure that an instrument remains within the required performance specification;
- c) *in situ* checks, i.e. a minimum level of testing required to indicate that an instrument is likely to be functioning within the required performance specification.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 2631-1, *Mechanical vibration and shock — Evaluation of human exposure to whole-body vibration — Part 1: General requirements*

ISO 2631-2, *Mechanical vibration and shock — Evaluation of human exposure to whole-body vibration — Part 2: Vibration in buildings (1 Hz to 80 Hz)*

ISO 2631-4:2001, *Mechanical vibration and shock — Evaluation of human exposure to whole-body vibration — Part 4: Guidelines for the evaluation of the effects of vibration and rotational motion on passenger and crew comfort in fixed-guideway transport systems*

ISO 5347 (all parts), *Methods for the calibration of vibration and shock pick-ups*

ISO 5348, *Mechanical vibration and shock — Mechanical mounting of accelerometers*

ISO 5349-1:2001, *Mechanical vibration — Measurement and evaluation of human exposure to hand-transmitted vibration — Part 1: General requirements*

ISO 16063 (all parts), *Methods for the calibration of vibration and shock transducers*

ISO/IEC Guide 98-3, *Uncertainty of measurement — Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*

IEC 61000-4-2:2008, *Electromagnetic compatibility (EMC) — Part 4-2: Testing and measurement techniques – Electrostatic discharge immunity test*

IEC 61000-4-3:2006, *Electromagnetic compatibility (EMC) — Part 4-3: Testing and measurement techniques – Radiated, radio-frequency, electromagnetic field immunity test*

IEC 61000-4-6, *Electromagnetic compatibility (EMC) — Part 4-6: Testing and measurement techniques – Immunity to conducted disturbances, induced by radio-frequency fields*

IEC 61000-6-2:2005, *Electromagnetic compatibility (EMC) — Part 6-2: Generic standards – Immunity for industrial environments*

CISPR 22:2008, *Information technology equipment — Radio disturbance characteristics — Limits and methods of measurement*

3 Terms, definitions and symbols

3.1 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 2041, ISO/IEC Guide 99 and the following apply.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <http://www.iso.org/obp>

3.1.1 General

3.1.1.1 vibration acceleration

component of acceleration, where the axis of measurement is specified by application standards

3.1.1.2 band-limiting frequency weighting

component of a frequency weighting defined by the high- and low-pass band-limiting filters

3.1.1.3 band-limited frequency range

frequency range defined by the band-limiting component of a frequency weighting

3.1.1.4 nominal frequency range

frequency range of interest, as defined in the relevant measurement standard

3.1.1.5**linear operating range**

range between lower and upper boundaries, on each measurement range, over which the linearity errors do not exceed the applicable tolerance limits specified in this document

3.1.1.6**overload**

condition that occurs when the upper boundary of the linear operating range is exceeded

3.1.1.7**under-range**

condition that occurs when the vibration value is below the lower boundary of the linear operating range

3.1.1.8**reference measurement range**

level range specified for testing the characteristics of the vibration instrumentation

Note 1 to entry: This range is used for measuring the reference vibration.

3.1.1.9**reference vibration signal**

sinusoidal vibration signal, the magnitude and frequency of which are specified in this document for testing the electromechanical performance of a human-vibration meter

Note 1 to entry: Different reference vibration signals are specified according to the application of the instrumentation.

3.1.1.10**calibration check frequency**

frequency specified for providing a check of the vibration sensitivity of the instrument

3.1.1.11**tone burst**

one or more complete cycles of a sinusoidal signal that start and end at a zero crossing of the waveform

3.1.1.12**signal burst**

one or more complete cycles of a periodic signal (such as saw tooth) that start and end at a zero crossing of the waveform

3.1.1.13**vibration measuring instrumentation**

combination of a vibration transducer, signal processor and display, being any single instrument, or a collection of instruments, which is/are capable of measuring parameters relating to human response to vibration

Note 1 to entry: See [Figures 1](#) and [2](#).

3.1.1.14**instrument documentation**

instruction manual, operating procedure or other documentation provided for the use of users of the vibration measurement instrument

3.1.2 Frequency-weighted values

3.1.2.1

time-averaged weighted acceleration value

frequency-weighted root-mean-square (r.m.s.) vibration acceleration value in a specified axis, a_w , in metres per second squared or radians per second squared, as defined by the expression

$$a_w = \left(\frac{1}{T} \int_0^T a_w^2(\xi) d\xi \right)^{1/2}$$

where

$a_w(\xi)$ is the translational or rotational, frequency-weighted vibration acceleration in a specified direction or around a specified axis as a function of the instantaneous time, ξ in metres per second squared (m/s^2) or radians per second squared (rad/s^2), respectively;

T is the duration of the measurement.

3.1.2.2

time-averaged weighted acceleration level

frequency-weighted r.m.s. vibration acceleration level expressed in decibels, as defined by

$$L_w = 20 \lg \frac{a_w}{a_0} \text{ dB}$$

where

a_w is the frequency-weighted r.m.s. acceleration value;

a_0 is the reference acceleration (in ISO 1683 for translational acceleration defined as 10^{-6} m/s^2).

3.1.2.3

running r.m.s. acceleration value

frequency-weighted running r.m.s. vibration acceleration, in metres per second squared, defined by the expression

$$a_{w,\theta}(t) = \left(\frac{1}{\theta} \int_{t-\theta}^t a_w^2(\xi) d\xi \right)^{1/2}$$

where

$a_w(\xi)$ is the frequency-weighted instantaneous vibration acceleration at time ξ , in metres per second squared or radians per second squared (rad/s^2), respectively;

θ is the integration time of the measurement;

t is the instantaneous time.

Note 1 to entry: Exponential averaging may be used for the running r.m.s. method, as an approximation of the linear averaging. The exponential averaging is defined as follows:

$$a_{w,\tau}(t) = \left(\frac{1}{\tau} \int_{-\infty}^t a_w^2(\xi) \exp\left(\frac{\xi-t}{\tau}\right) d\xi \right)^{1/2}$$

where τ is the time constant.

3.1.2.4**maximum transient vibration value****MTVV**

maximum value of the running r.m.s. vibration acceleration value when the integration time is equal to 1 s

3.1.2.5**motion sickness dose value****MSDV**

integral of the squared frequency-weighted instantaneous vibration acceleration $a_w(t)$ in $\text{m/s}^{1,5}$ as defined by the expression

$$\text{MSDV} = \left(\int_0^{\Phi} a_w^2(\xi) d\xi \right)^{1/2}$$

where Φ is the total period during which motion could occur

Note 1 to entry: The motion sickness dose value can be obtained from the frequency-weighted r.m.s. vibration acceleration through multiplication by $\Phi^{1/2}$.

Note 2 to entry: For measurement instrumentation, the exposure period, Φ , is likely to be assumed to be equal to the measurement period, T , unless otherwise indicated.

3.1.2.6**vibration dose value****VDV**

integral of the fourth power of the frequency-weighted instantaneous vibration acceleration $a_w(t)$ in $\text{m/s}^{1,75}$ as defined by the expression

$$\text{VDV} = \left(\int_0^{\Phi} a_w^4(\xi) d\xi \right)^{1/4}$$

where Φ is the total (daily) period for which vibration exposure occurs

Note 1 to entry: The vibration dose value is more sensitive to peaks than is the r.m.s. value.

Note 2 to entry: For measurement instrumentation, the exposure period, Φ , is likely to be assumed to be equal to the measurement period, T , unless otherwise indicated.

3.1.2.7**vibration total value**

combined vibration from three axes of translational vibration, as defined by the expression

$$a_{wv} = \sqrt{k_x^2 a_{wx}^2 + k_y^2 a_{wy}^2 + k_z^2 a_{wz}^2}$$

where

a_{wx} , a_{wy} and a_{wz} are the weighted vibration values in the three orthogonal axes x , y and z ;

k_x , k_y and k_z are multiplying constants whose values depend on the measurement application

3.1.2.8**peak vibration value**

maximum modulus of the instantaneous (positive and negative) peak values of the frequency-weighted acceleration

3.1.2.9

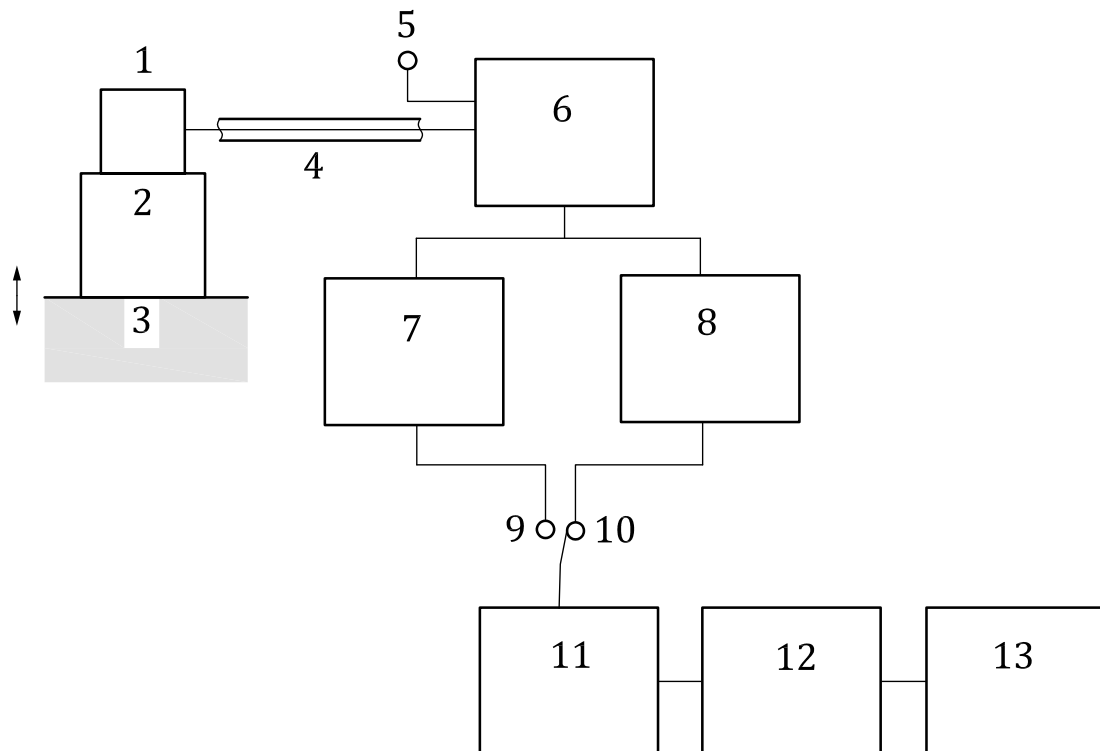
crest factor

parameter for a measurement period, given by the peak vibration value divided by the r.m.s. vibration value, with both values having the same frequency weighting

3.2 Symbols

For the purposes of this document, the following symbols and abbreviated terms apply.

a_w	time-averaged frequency-weighted single-axis vibration acceleration
$a_w(t), a_w(\xi)$	instantaneous frequency-weighted translational or rotational single-axis acceleration at time t , or time ξ
f	frequency
H	overall frequency weighting function
k_i	multiplying constants applied to the whole-body frequency-weighted acceleration value for axis i
n	one-third-octave band number
s	variable of the Laplace transform
t or ξ	instantaneous time
T	measurement duration
W_x	frequency weighting
Φ	exposure duration
$\Delta P_{\max}$	maximum peak value deviation
$\Delta\varphi$	phase error
$\Delta\vartheta$	phase delay time difference
τ	exponential averaging time constant
θ	linear averaging time
MSDV	motion sickness dose value
MTVV	maximum transient vibration value
VDV	vibration dose value

**Key**

- | | | | |
|---|---------------------|----|---|
| 1 | transducer | 8 | frequency weighting — including band-limiting |
| 2 | mounting system | 9 | band-limited output |
| 3 | vibrating surface | 10 | frequency-weighted output |
| 4 | cable | 11 | time weighting |
| 5 | electrical input | 12 | additional processing |
| 6 | signal conditioning | 13 | display |
| 7 | band limiting | | |

Figure 1 — Example of the basic functional path of a vibration measurement instrument or measurement system — time-domain signal processing